

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026520.D
 Acq On : 23 Jun 2022 17:32
 Operator : SY/MD
 Sample : N3425-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.262	53	69	70	rBV7	14314	23526	3.34%	0.413%
2	1.317	80	86	102	rVB	131376	143938	20.41%	2.530%
3	1.577	160	167	180	rBV	107500	128631	18.24%	2.261%
4	2.117	325	335	354	rVB	227510	334002	47.36%	5.870%
5	2.304	386	393	405	rVB2	5606	9336	1.32%	0.164%
6	3.931	886	899	934	rBV2	35867	164443	23.32%	2.890%
7	4.358	1015	1032	1061	rBV2	129544	346645	49.15%	6.092%
8	5.056	1233	1249	1282	rBV2	284449	705300	100.00%	12.395%
9	5.622	1414	1425	1453	rBV	230552	473863	67.19%	8.328%
10	6.075	1551	1566	1591	rBV	155552	328396	46.56%	5.771%
11	6.583	1709	1724	1739	rBV4	11475	28056	3.98%	0.493%
12	6.992	1840	1851	1880	rBV	52665	100580	14.26%	1.768%
13	7.146	1887	1899	1908	rBV5	6270	12602	1.79%	0.221%
14	7.317	1940	1952	1970	rBV	334680	587756	83.33%	10.329%
15	7.400	1970	1978	1991	rVB	13300	27146	3.85%	0.477%
16	7.628	2038	2049	2063	rBV2	27341	50736	7.19%	0.892%
17	7.940	2130	2146	2155	rBV2	8908	16186	2.29%	0.284%
18	8.095	2184	2194	2243	rBV2	216189	458307	64.98%	8.054%
19	8.853	2418	2430	2449	rBV	347574	571193	80.99%	10.038%
20	9.146	2507	2521	2532	rBV6	5684	12801	1.81%	0.225%
21	10.217	2840	2854	2872	rBV	107469	169968	24.10%	2.987%
22	10.381	2893	2905	2917	rBV	24943	39742	5.63%	0.698%
23	11.249	3164	3175	3196	rBV	312538	491012	69.62%	8.629%
24	11.622	3278	3291	3311	rBV	286014	450623	63.89%	7.919%
25	12.249	3478	3486	3496	rVB2	5099	7553	1.07%	0.133%
26	16.487	4798	4804	4812	rVB6	5631	7737	1.10%	0.136%




Sum of corrected areas: 5690078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026520.D
Acq On : 23 Jun 2022 17:32
Operator : SY/MD
Sample : N3425-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

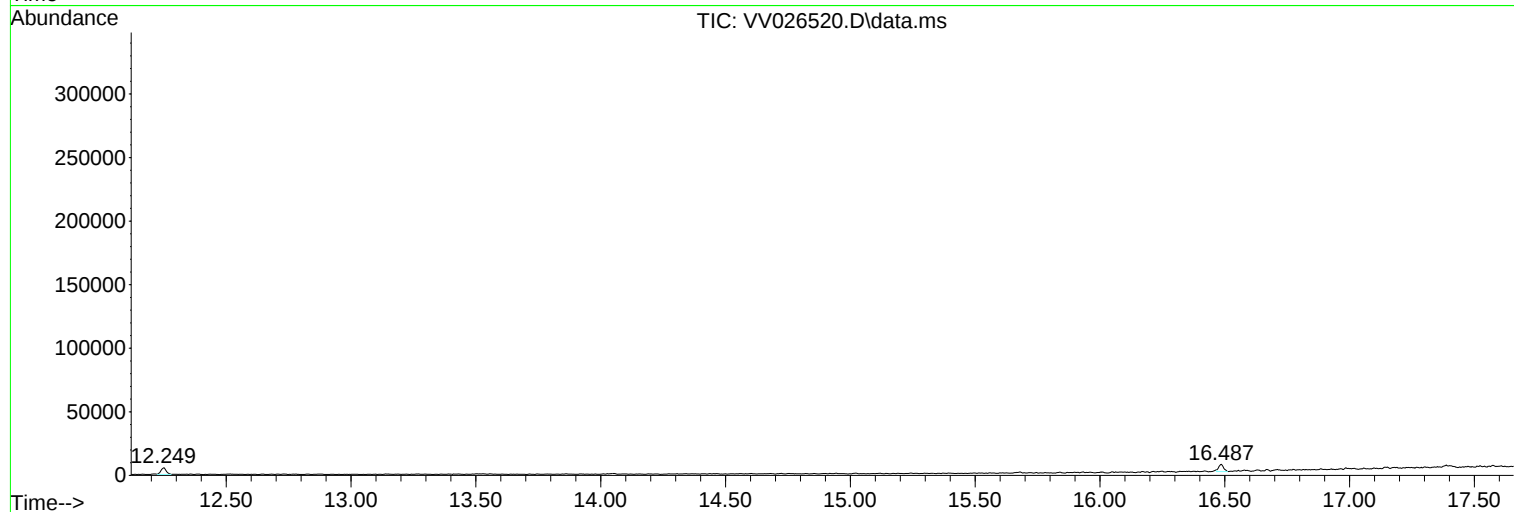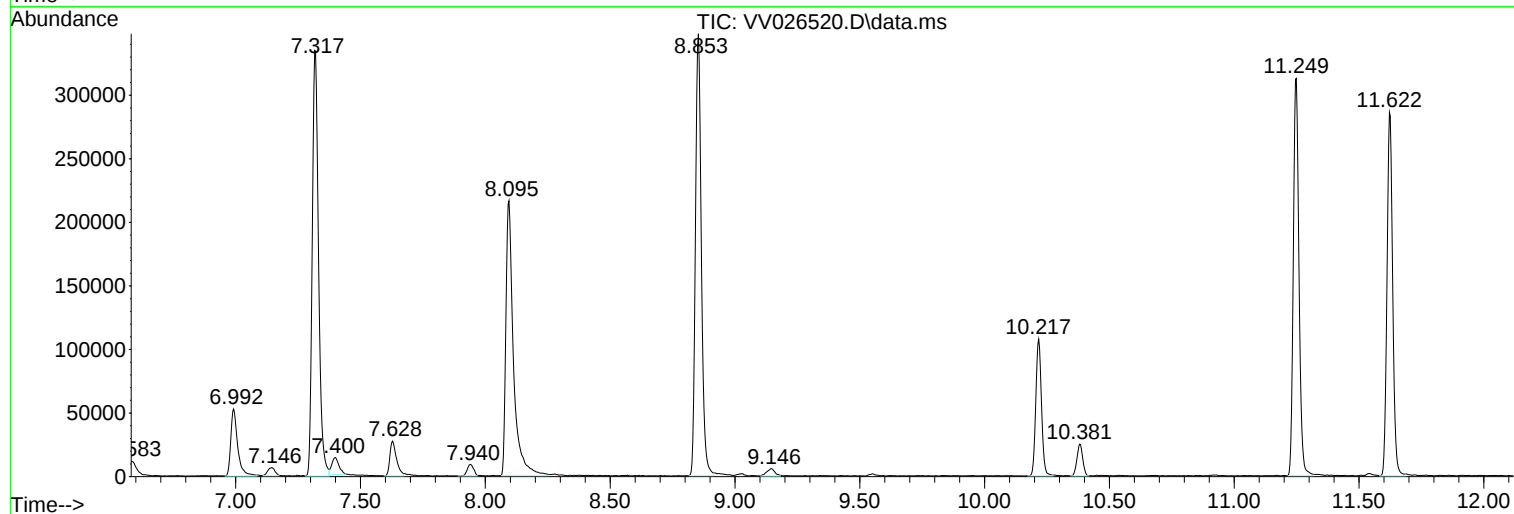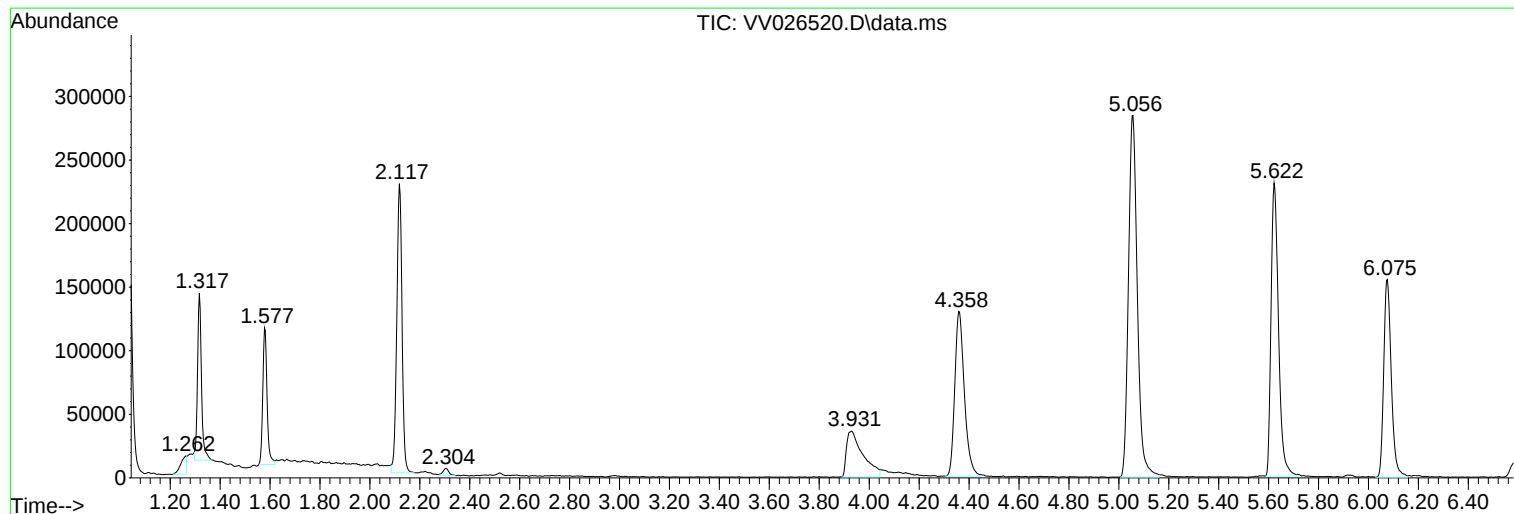

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026520.D
Acq On : 23 Jun 2022 17:32
Operator : SY/MD
Sample : N3425-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026520.D
Acq On : 23 Jun 2022 17:32
Operator : SY/MD
Sample : N3425-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc