

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026521.D
 Acq On : 23 Jun 2022 17:56
 Operator : SY/MD
 Sample : N3401-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	55	73	78	rBV	16028	50293	7.57%	0.935%
2	1.317	79	86	99	rVB	124469	143872	21.65%	2.674%
3	1.577	160	167	178	rBV	102193	117235	17.64%	2.179%
4	2.117	325	335	353	rVB	211128	312899	47.08%	5.814%
5	3.921	883	896	942	rBV3	42915	209244	31.48%	3.888%
6	4.358	1013	1032	1062	rBV2	119244	299549	45.07%	5.566%
7	5.053	1233	1248	1275	rBV2	272172	664640	100.00%	12.351%
8	5.622	1410	1425	1454	rBV	229322	464783	69.93%	8.637%
9	6.072	1541	1565	1591	rBV	151255	314117	47.26%	5.837%
10	6.992	1841	1851	1873	rBV	46563	89405	13.45%	1.661%
11	7.316	1941	1952	1971	rBV	312887	542954	81.69%	10.090%
12	7.397	1973	1977	1996	rVB2	6708	13718	2.06%	0.255%
13	7.628	2038	2049	2071	rBV	23610	45448	6.84%	0.845%
14	7.940	2136	2146	2159	rVB2	7166	13639	2.05%	0.253%
15	8.091	2184	2193	2239	rBV	203644	440722	66.31%	8.190%
16	8.853	2418	2430	2455	rBV	332764	556026	83.66%	10.332%
17	10.217	2843	2854	2877	rBV2	102492	162105	24.39%	3.012%
18	10.381	2893	2905	2917	rBV2	21798	35714	5.37%	0.664%
19	11.249	3161	3175	3197	rBV	301355	474548	71.40%	8.818%
20	11.622	3279	3291	3310	rBV	273363	423141	63.66%	7.863%
21	12.249	3476	3486	3499	rVB	4447	7320	1.10%	0.136%




Sum of corrected areas: 5381372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026521.D
Acq On : 23 Jun 2022 17:56
Operator : SY/MD
Sample : N3401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

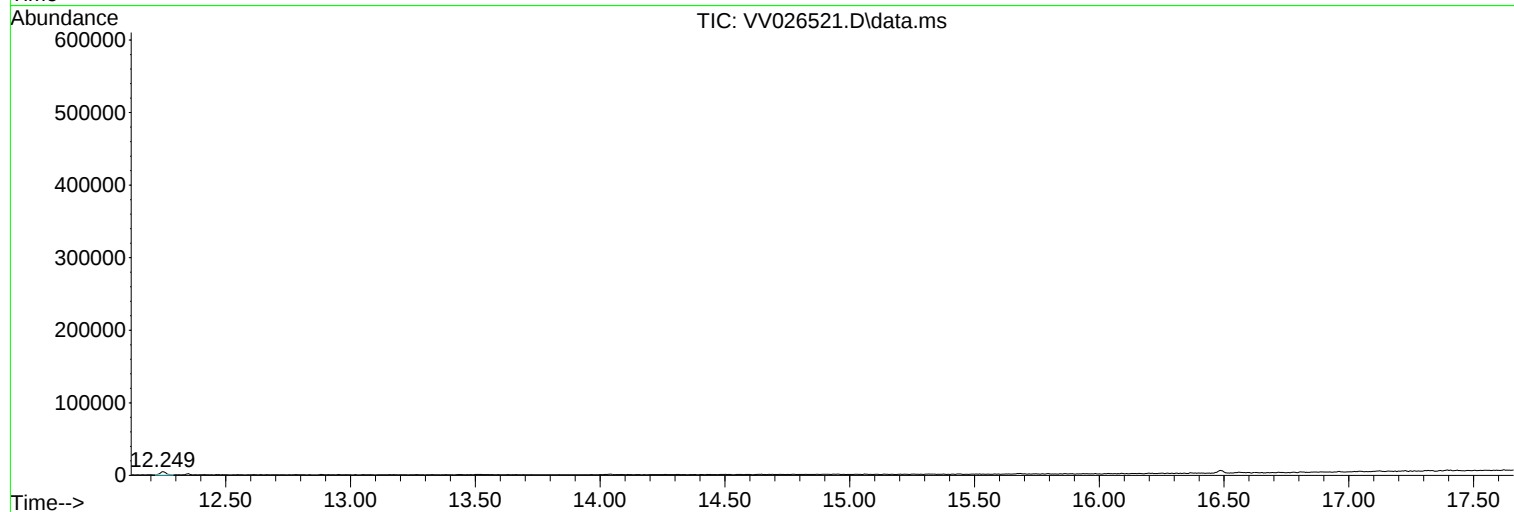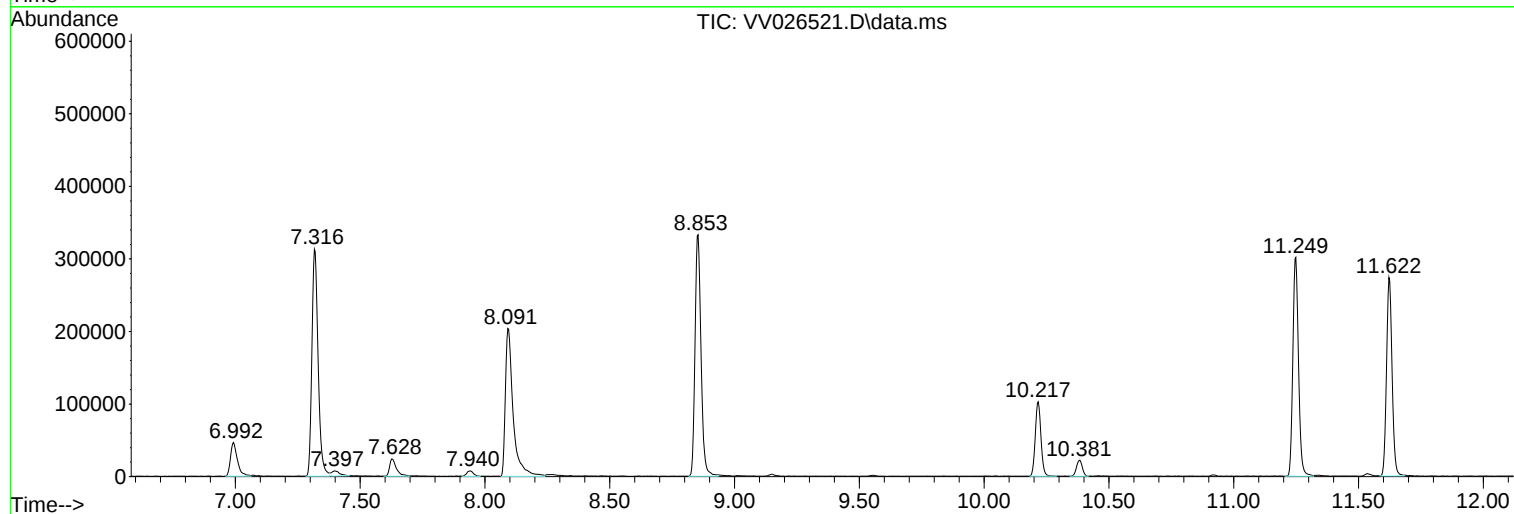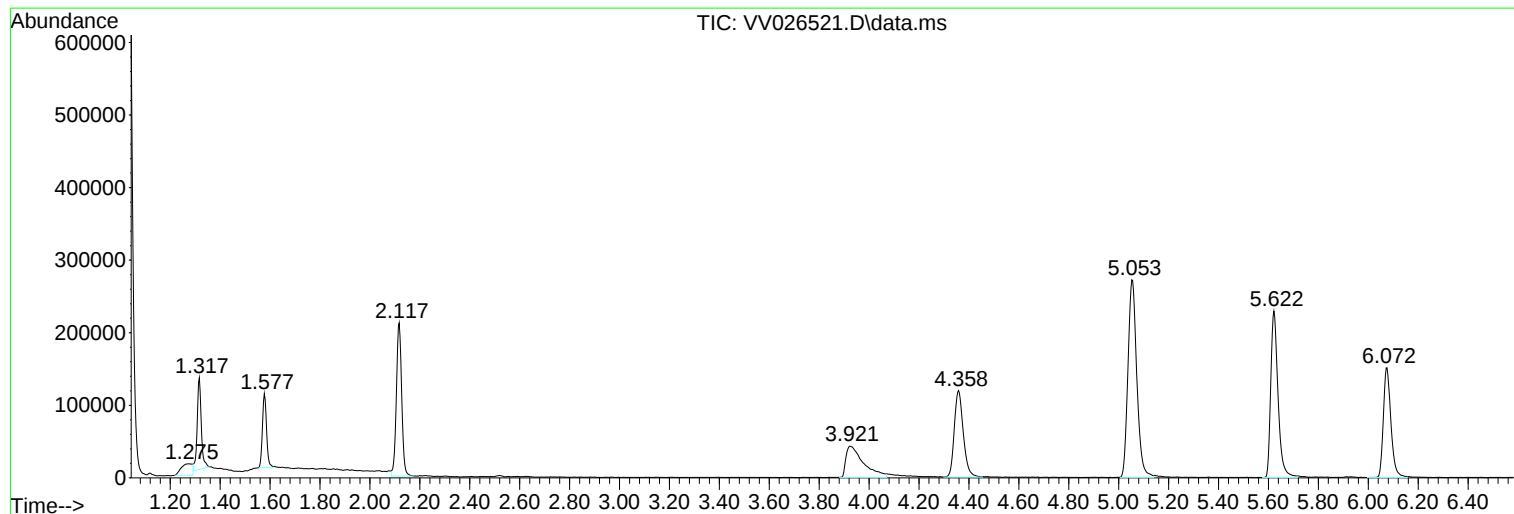

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026521.D
Acq On : 23 Jun 2022 17:56
Operator : SY/MD
Sample : N3401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026521.D
Acq On : 23 Jun 2022 17:56
Operator : SY/MD
Sample : N3401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
