

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026522.D
 Acq On : 23 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3401-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	53	73	74	rBV4	13570	31791	4.72%	0.596%
2	1.317	79	86	108	rVB	130821	158546	23.53%	2.971%
3	1.577	160	167	178	rVV	102368	119965	17.81%	2.248%
4	2.117	325	335	353	rVB	214505	315213	46.79%	5.906%
5	2.304	385	393	405	rVB	11060	17091	2.54%	0.320%
6	3.921	886	896	934	rBV3	35187	168674	25.04%	3.161%
7	4.358	1015	1032	1073	rVB	119845	302813	44.95%	5.674%
8	5.053	1230	1248	1288	rBV2	270738	673729	100.00%	12.624%
9	5.622	1413	1425	1454	rBV	223708	457964	67.97%	8.581%
10	6.075	1552	1566	1589	rBV	152224	313898	46.59%	5.882%
11	6.992	1839	1851	1873	rBV	45847	88767	13.18%	1.663%
12	7.317	1938	1952	1972	rBV	307434	547970	81.33%	10.268%
13	7.397	1973	1977	2001	rVB2	7792	16046	2.38%	0.301%
14	7.628	2039	2049	2063	rBV2	24903	44847	6.66%	0.840%
15	7.940	2134	2146	2156	rBV2	6519	11313	1.68%	0.212%
16	8.095	2184	2194	2230	rBV	200508	425653	63.18%	7.976%
17	8.853	2418	2430	2461	rBV	330320	548372	81.39%	10.275%
18	9.143	2513	2520	2533	rBV3	6826	11198	1.66%	0.210%
19	10.217	2843	2854	2872	rBV	101164	162535	24.12%	3.046%
20	10.381	2893	2905	2917	rBV2	19196	30057	4.46%	0.563%
21	11.249	3163	3175	3194	rBV	299138	466868	69.30%	8.748%
22	11.622	3279	3291	3309	rBV	273314	423482	62.86%	7.935%




Sum of corrected areas: 5336792

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026522.D
Acq On : 23 Jun 2022 18:20
Operator : SY/MD
Sample : N3401-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

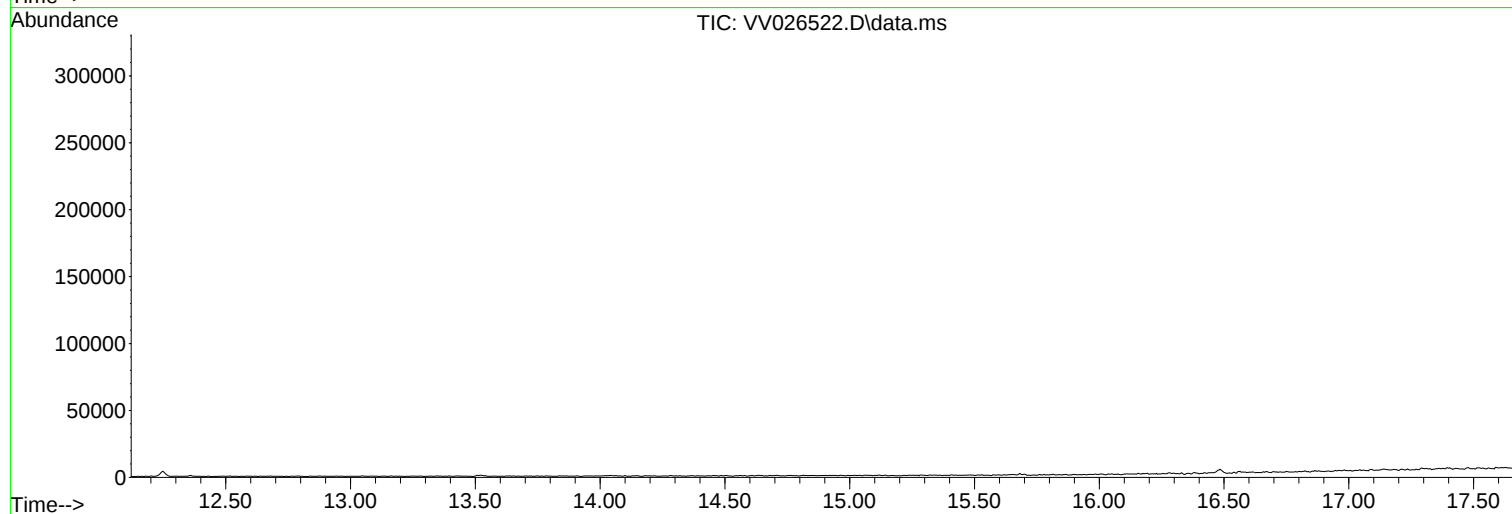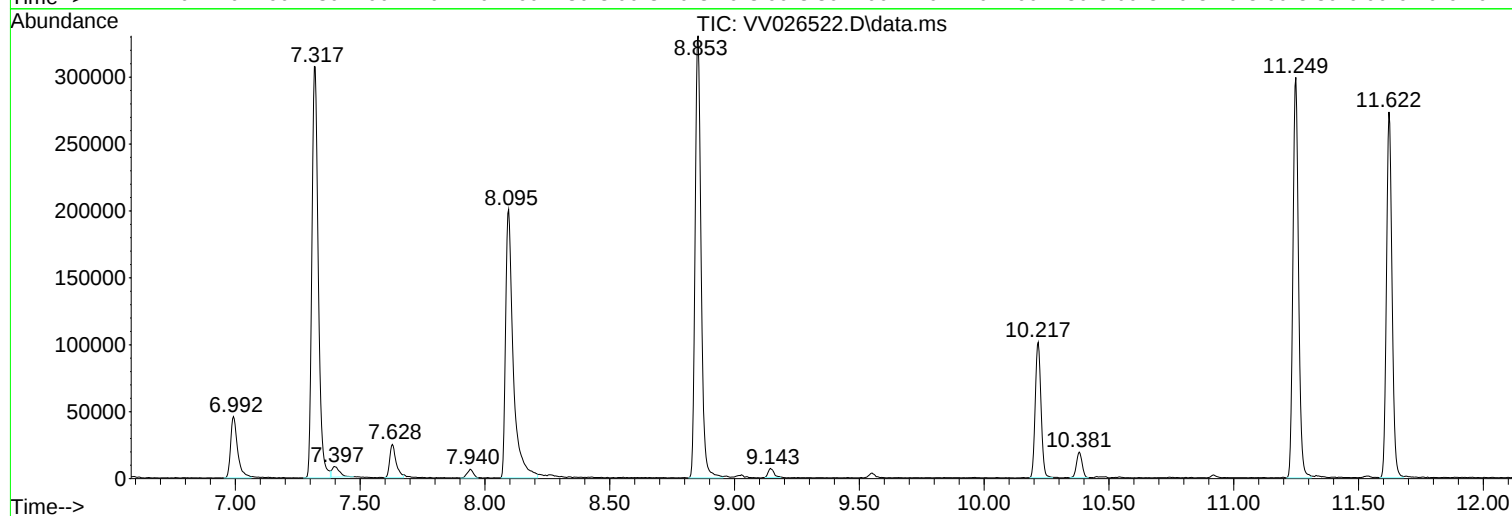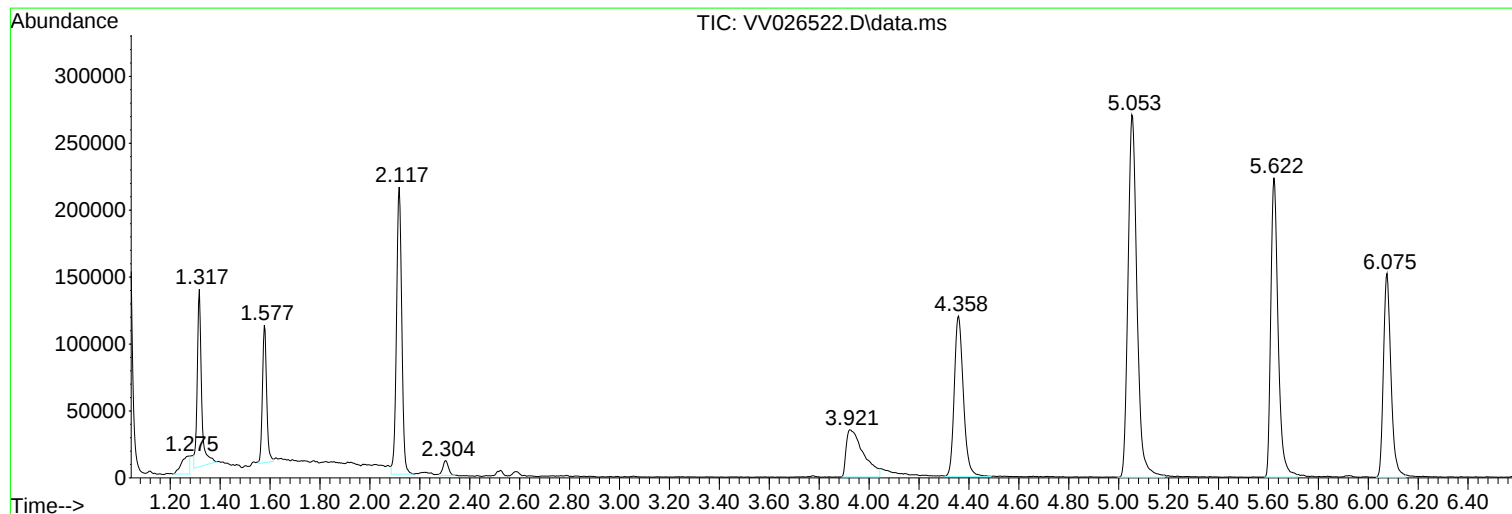

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026522.D
Acq On : 23 Jun 2022 18:20
Operator : SY/MD
Sample : N3401-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026522.D
Acq On : 23 Jun 2022 18:20
Operator : SY/MD
Sample : N3401-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
