

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026528.D
 Acq On : 23 Jun 2022 20:43
 Operator : SY/MD
 Sample : N3400-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	40	rVB2	15988	17867	3.00%	0.356%
2	1.253	52	66	70	rBV4	17581	30452	5.11%	0.608%
3	1.317	79	86	99	rVB	91374	105013	17.64%	2.095%
4	1.426	115	120	134	rVB	28708	35982	6.04%	0.718%
5	1.577	160	167	179	rBV	74916	93509	15.71%	1.866%
6	2.118	326	335	354	rVB	155468	227473	38.21%	4.538%
7	2.307	386	394	404	rVB	11026	16819	2.83%	0.336%
8	2.519	451	460	473	rVB2	5380	9725	1.63%	0.194%
9	3.191	657	669	685	rBV2	6716	14492	2.43%	0.289%
10	3.928	883	898	935	rBV2	40373	190566	32.01%	3.802%
11	4.359	1016	1032	1062	rVB	106250	265214	44.55%	5.291%
12	5.056	1232	1249	1283	rBV2	237247	595350	100.00%	11.877%
13	5.622	1413	1425	1456	rBV	195059	399809	67.16%	7.976%
14	6.076	1552	1566	1590	rBV	130746	275244	46.23%	5.491%
15	6.995	1841	1852	1872	rBV	34701	67601	11.35%	1.349%
16	7.317	1941	1952	1967	rVV	269379	471484	79.19%	9.406%
17	7.394	1967	1976	1996	rVB	67671	127851	21.47%	2.551%
18	7.629	2041	2049	2070	rBV2	18040	33886	5.69%	0.676%
19	8.095	2183	2194	2228	rBV3	188221	409353	68.76%	8.167%
20	8.854	2419	2430	2451	rBV	287062	479106	80.47%	9.558%
21	9.021	2472	2482	2491	rBV2	7531	11686	1.96%	0.233%
22	9.140	2510	2519	2535	rBV3	19860	34847	5.85%	0.695%
23	9.548	2635	2646	2657	rBV	17728	28992	4.87%	0.578%
24	10.217	2843	2854	2866	rBV	91574	146633	24.63%	2.925%
25	10.381	2890	2905	2915	rBV4	4959	9639	1.62%	0.192%
26	10.452	2917	2927	2933	rBV2	5425	8379	1.41%	0.167%
27	10.915	3060	3071	3086	rBV	17135	25485	4.28%	0.508%
28	11.249	3163	3175	3191	rBV	267804	420783	70.68%	8.395%
29	11.336	3195	3202	3212	rVB2	9798	14458	2.43%	0.288%
30	11.535	3253	3264	3280	rBV3	11573	22666	3.81%	0.452%
31	11.622	3280	3291	3316	rVB	247198	397381	66.75%	7.928%
32	12.239	3474	3483	3494	rBV5	3744	6589	1.11%	0.131%
33	13.323	3809	3820	3829	rBV2	5766	9021	1.52%	0.180%
34	16.178	4702	4708	4716	rVB7	6910	9121	1.53%	0.182%

Sum of corrected areas: 5012476




Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026528.D
Acq On : 23 Jun 2022 20:43
Operator : SY/MD
Sample : N3400-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

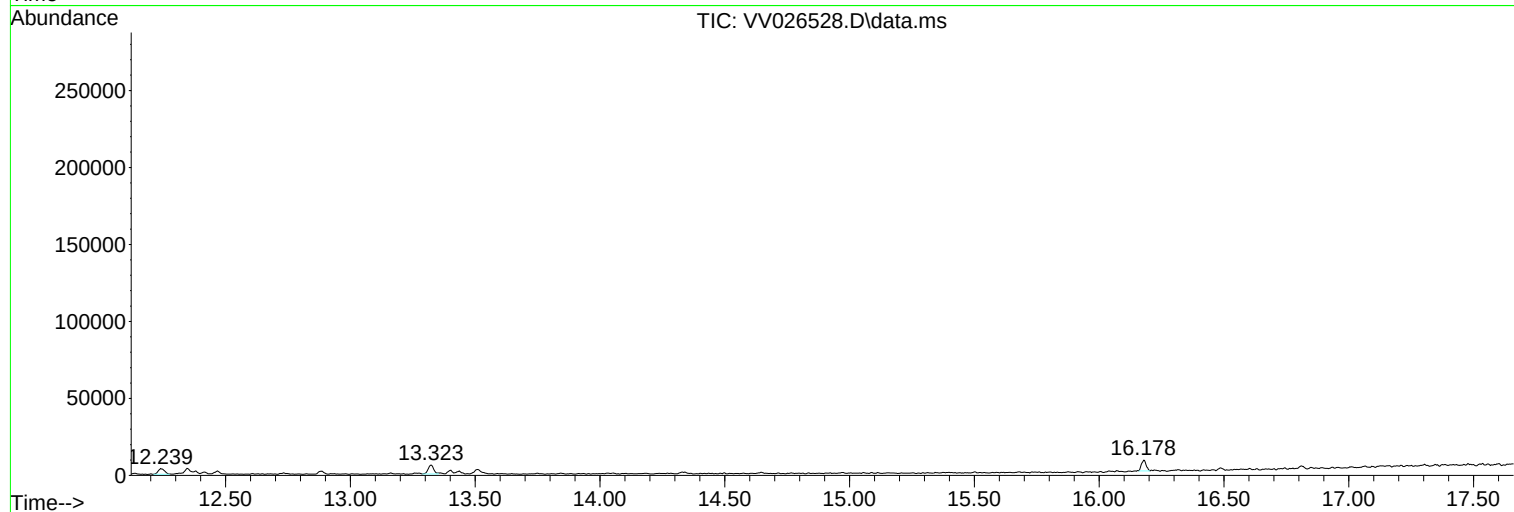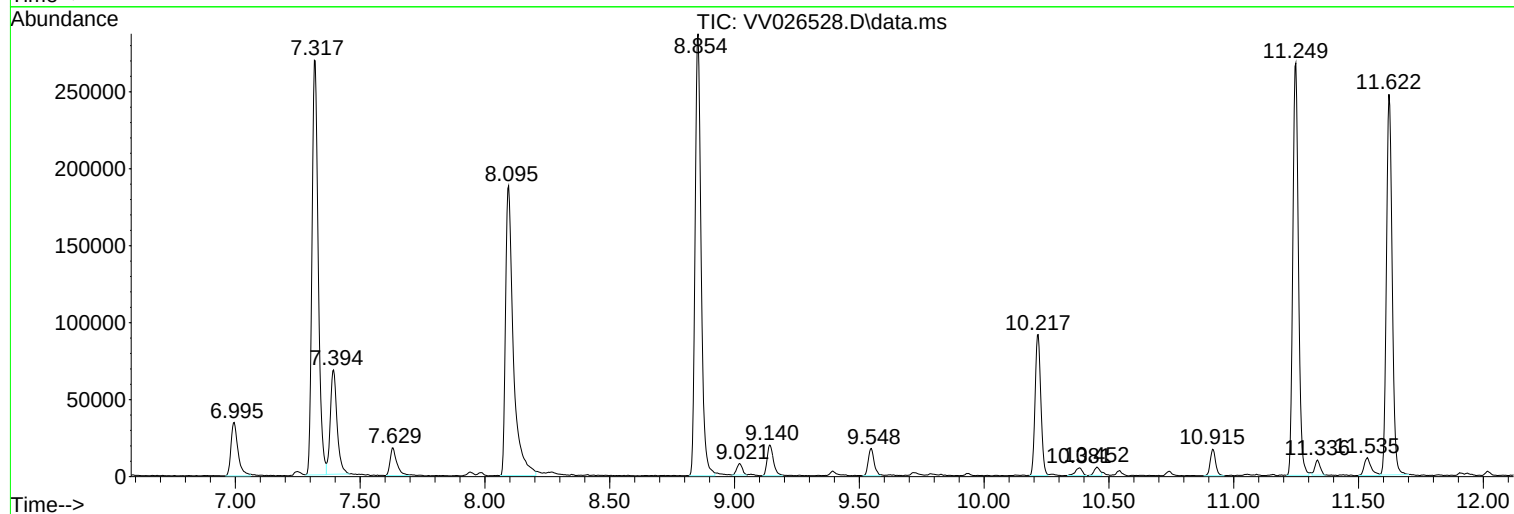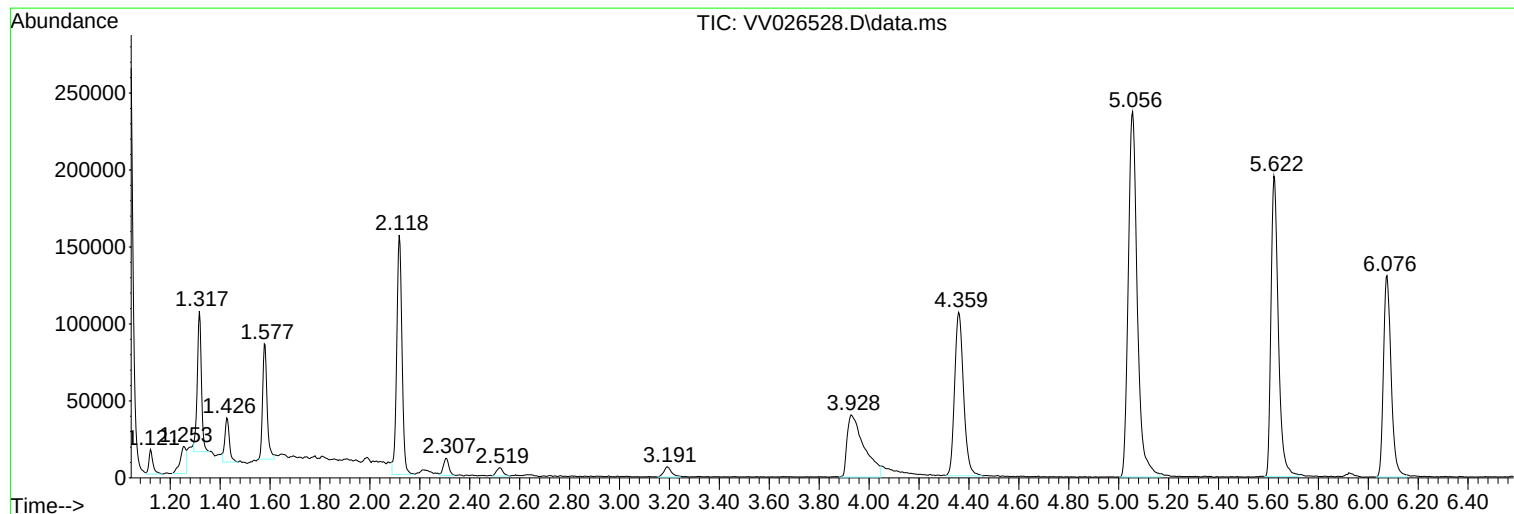

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026528.D
Acq On : 23 Jun 2022 20:43
Operator : SY/MD
Sample : N3400-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026528.D
Acq On : 23 Jun 2022 20:43
Operator : SY/MD
Sample : N3400-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc