

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026529.D
 Acq On : 23 Jun 2022 21:07
 Operator : SY/MD
 Sample : N3400-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	52	74	76	rBV2	16754	43768	7.91%	1.002%
2	1.317	80	86	105	rVB	82592	106461	19.25%	2.438%
3	1.577	160	167	183	rBV	74752	89430	16.17%	2.048%
4	2.117	326	335	352	rVB	146920	219176	39.63%	5.019%
5	3.928	884	898	934	rBV3	33563	160349	28.99%	3.672%
6	4.358	1016	1032	1064	rVB2	100661	254136	45.95%	5.820%
7	5.056	1233	1249	1282	rBV2	225628	553029	100.00%	12.664%
8	5.622	1414	1425	1459	rBV	185922	387225	70.02%	8.868%
9	6.075	1554	1566	1591	rBV	125092	262618	47.49%	6.014%
10	6.995	1839	1852	1878	rBV2	31151	62138	11.24%	1.423%
11	7.320	1941	1953	1970	rBV	250344	440269	79.61%	10.082%
12	7.400	1971	1978	1993	rVB2	11888	23517	4.25%	0.539%
13	7.632	2041	2050	2071	rBV4	16508	30782	5.57%	0.705%
14	8.095	2184	2194	2234	rBV2	178293	384347	69.50%	8.802%
15	8.853	2419	2430	2459	rBV	275738	458322	82.87%	10.496%
16	10.217	2843	2854	2870	rBV	88783	142238	25.72%	3.257%
17	10.381	2895	2905	2916	rBV2	6003	9861	1.78%	0.226%
18	11.249	3161	3175	3200	rBV	245739	383688	69.38%	8.787%
19	11.622	3280	3291	3313	rBV	224012	355432	64.27%	8.139%




Sum of corrected areas: 4366786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026529.D
Acq On : 23 Jun 2022 21:07
Operator : SY/MD
Sample : N3400-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

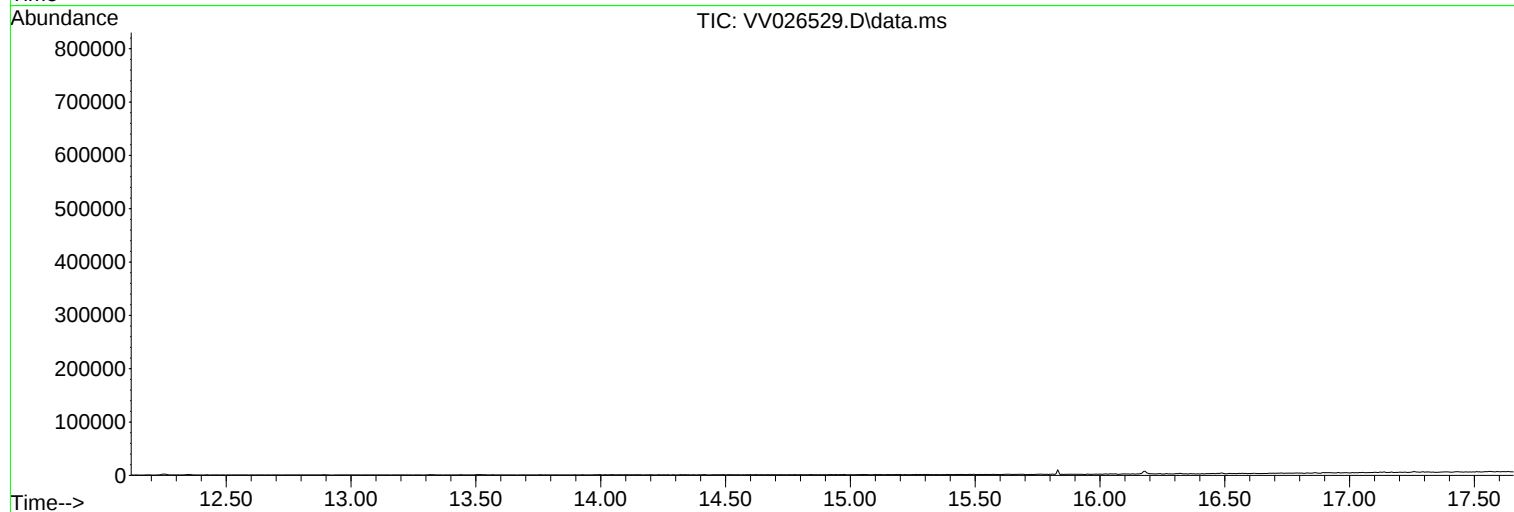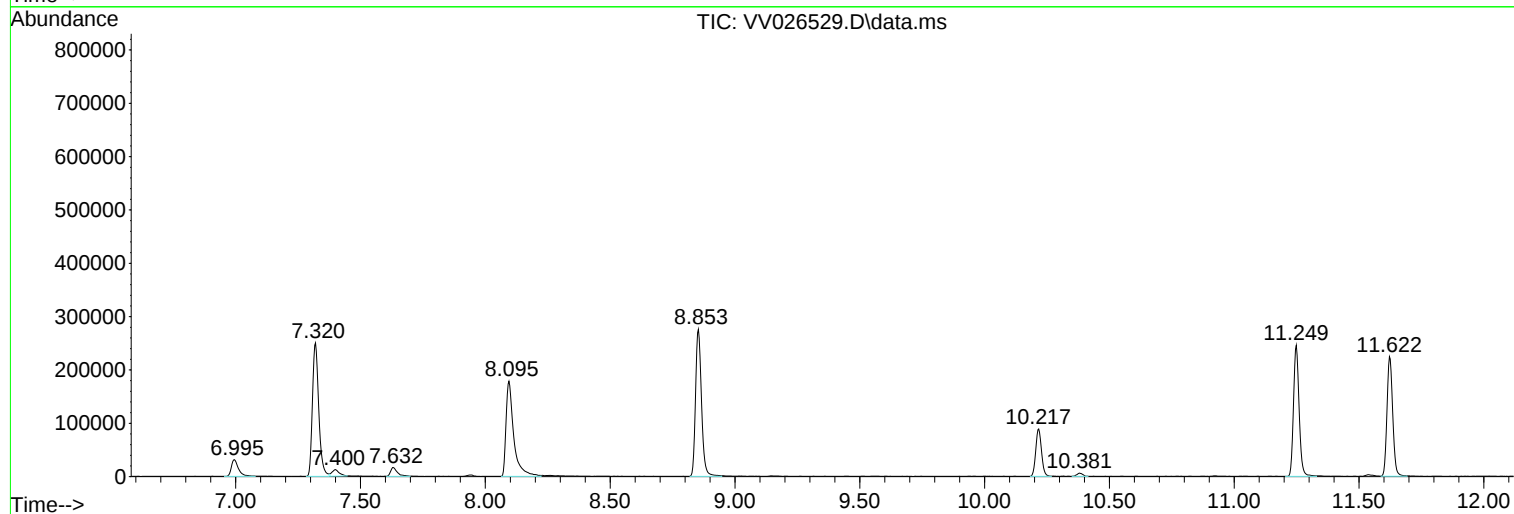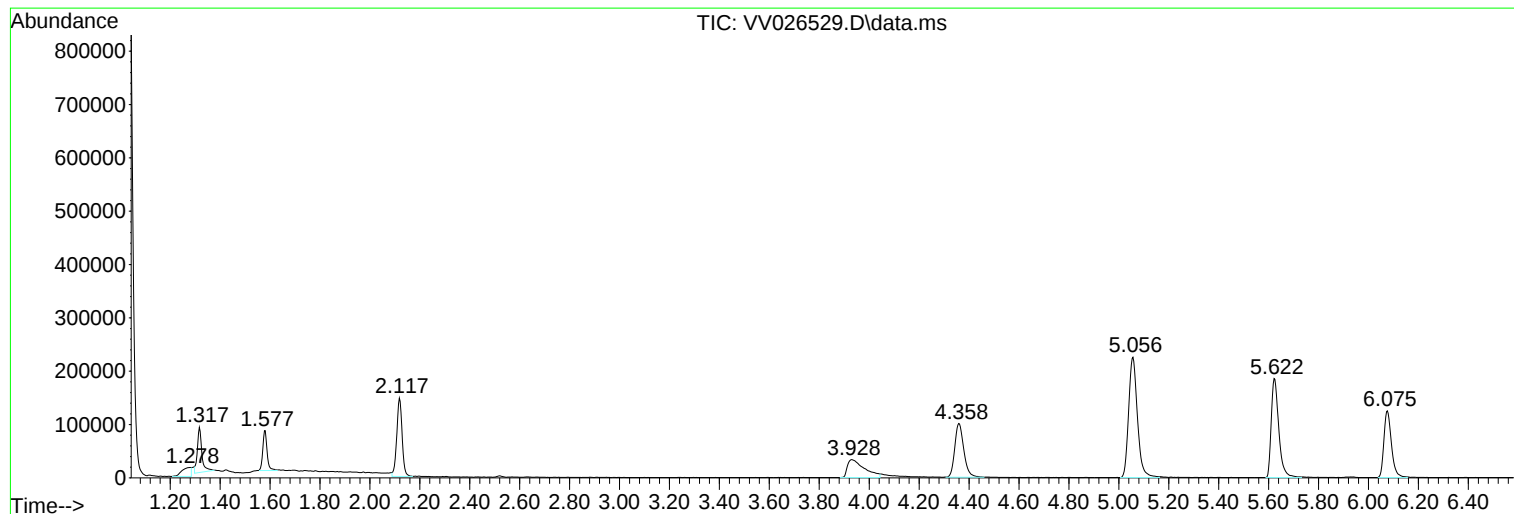

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026529.D
Acq On : 23 Jun 2022 21:07
Operator : SY/MD
Sample : N3400-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026529.D
Acq On : 23 Jun 2022 21:07
Operator : SY/MD
Sample : N3400-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc