

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026530.D
 Acq On : 23 Jun 2022 21:31
 Operator : SY/MD
 Sample : N3400-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	53	76	77	rBV3	15626	42951	7.87%	0.989%
2	1.317	80	86	101	rVB	77605	97394	17.85%	2.244%
3	1.580	161	168	176	rBV	71640	83034	15.22%	1.913%
4	2.117	326	335	355	rVB	145428	216658	39.72%	4.991%
5	3.928	884	898	940	rBV3	35240	173666	31.84%	4.000%
6	4.358	1017	1032	1063	rBV	99963	250453	45.91%	5.769%
7	5.056	1232	1249	1276	rBV2	221032	545480	100.00%	12.565%
8	5.625	1411	1426	1450	rBV	181338	379033	69.49%	8.731%
9	6.075	1554	1566	1592	rBV	127370	262811	48.18%	6.054%
10	6.995	1841	1852	1874	rBV	31859	62963	11.54%	1.450%
11	7.320	1940	1953	1969	rBV	244938	433366	79.45%	9.983%
12	7.397	1969	1977	1995	rVB	22767	45402	8.32%	1.046%
13	7.632	2038	2050	2069	rBV	17196	33100	6.07%	0.762%
14	8.095	2184	2194	2227	rBV2	175335	375890	68.91%	8.659%
15	8.853	2419	2430	2452	rBV	276929	455513	83.51%	10.493%
16	10.217	2842	2854	2869	rBV	89151	140760	25.80%	3.242%
17	10.381	2894	2905	2916	rVB2	7861	12373	2.27%	0.285%
18	11.249	3162	3175	3197	rBV	243897	381150	69.87%	8.780%
19	11.622	3280	3291	3312	rBV	220826	349118	64.00%	8.042%




Sum of corrected areas: 4341115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026530.D
Acq On : 23 Jun 2022 21:31
Operator : SY/MD
Sample : N3400-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

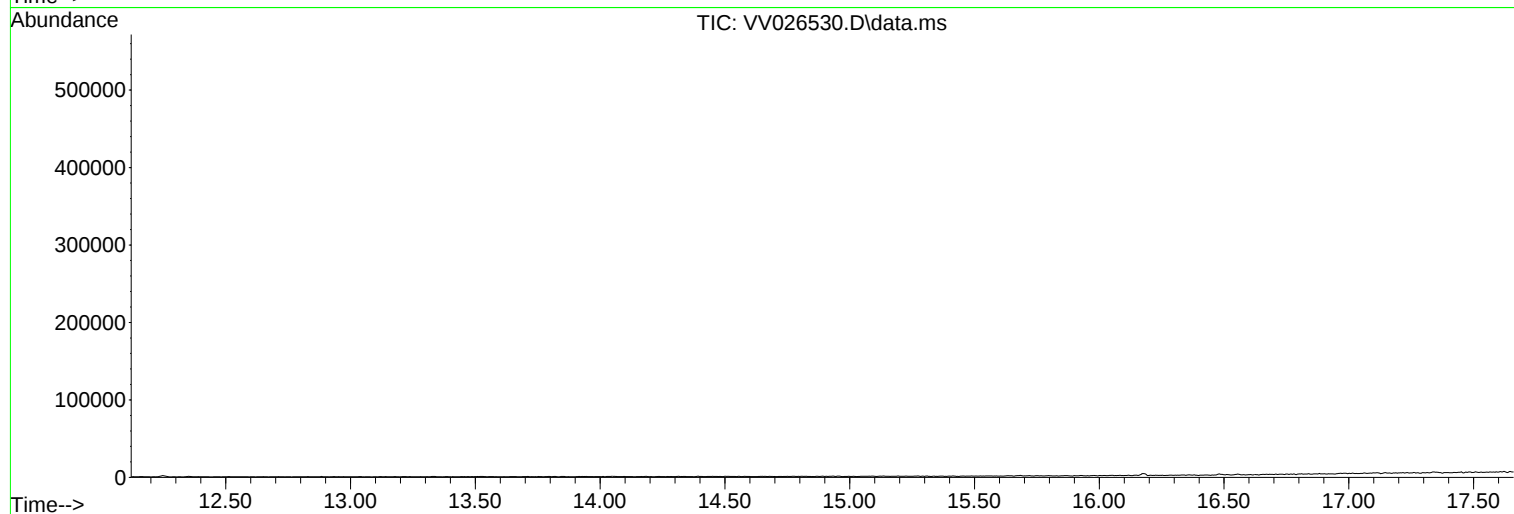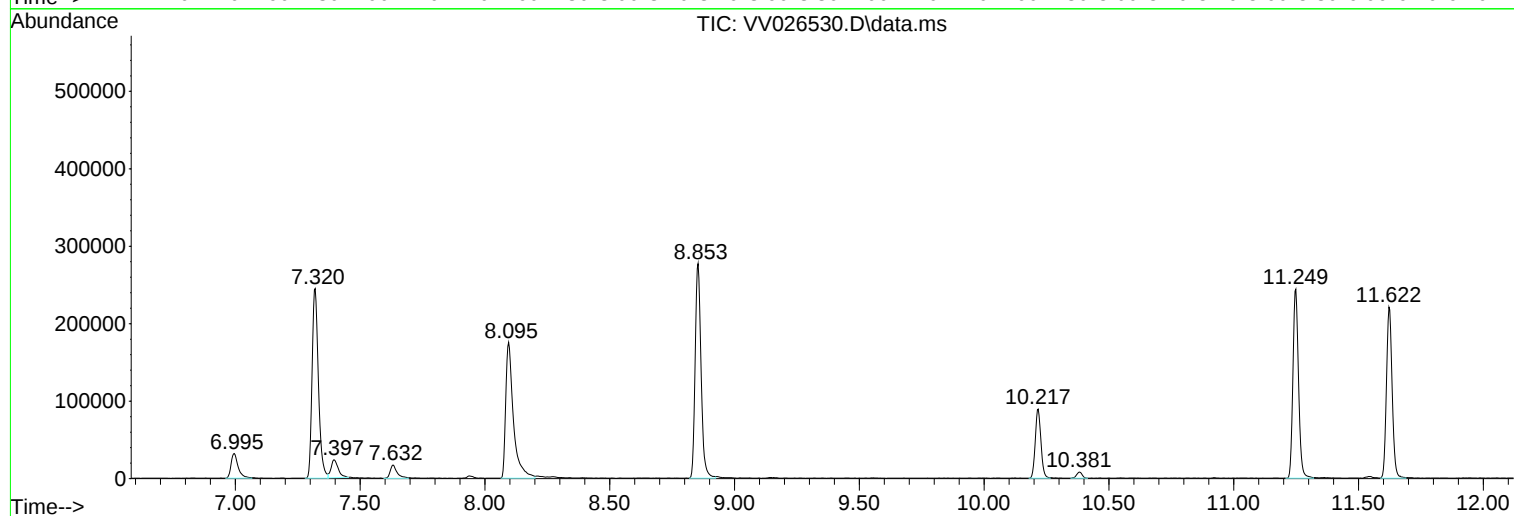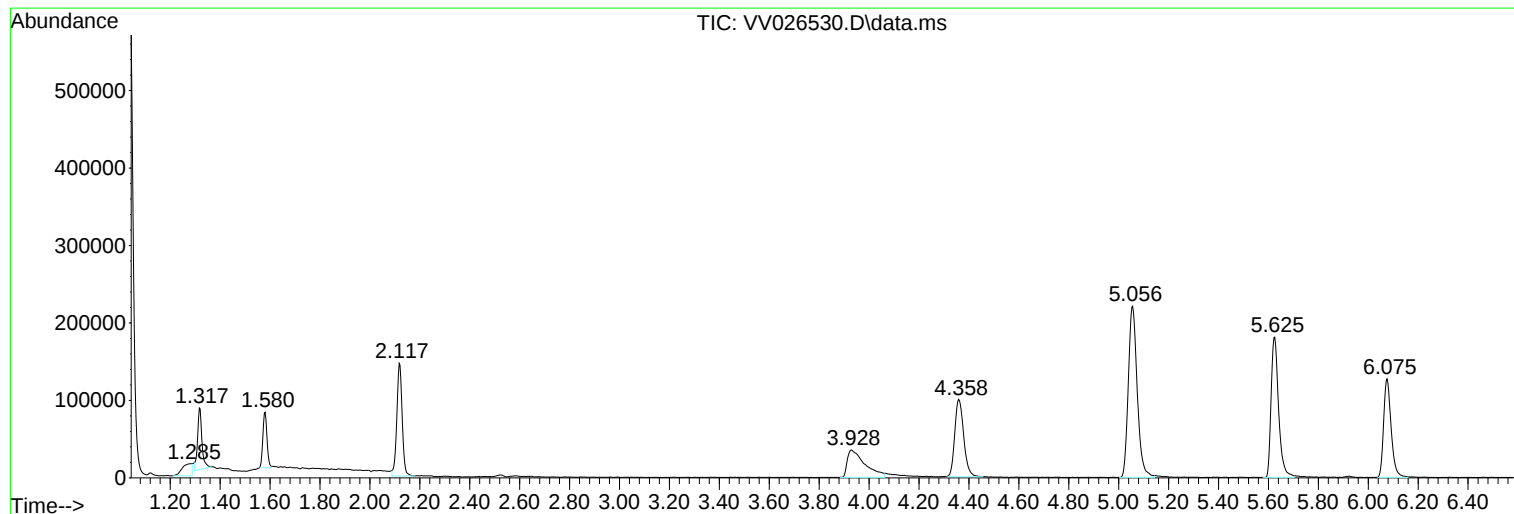

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026530.D
Acq On : 23 Jun 2022 21:31
Operator : SY/MD
Sample : N3400-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026530.D
Acq On : 23 Jun 2022 21:31
Operator : SY/MD
Sample : N3400-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc