

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026537.D
 Acq On : 24 Jun 2022 01:06
 Operator : SY/MD
 Sample : VV0623WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK384

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	53	73	76	rBV2	17167	42652	6.10%	0.761%
2	1.317	80	86	103	rVB	122536	147336	21.06%	2.628%
3	1.580	161	168	177	rBV	101123	115906	16.57%	2.068%
4	2.117	326	335	354	rVB	212904	320316	45.79%	5.714%
5	2.523	450	461	472	rVB4	5615	9770	1.40%	0.174%
6	3.931	884	899	950	rBV2	37887	186860	26.71%	3.334%
7	4.358	1016	1032	1060	rBV2	125499	314394	44.94%	5.609%
8	5.056	1233	1249	1284	rBV2	282944	699600	100.00%	12.481%
9	5.622	1407	1425	1453	rBV	249546	515280	73.65%	9.193%
10	6.075	1552	1566	1590	rBV	159390	328445	46.95%	5.859%
11	6.992	1837	1851	1878	rBV	47410	91301	13.05%	1.629%
12	7.320	1939	1953	1977	rBV	328317	584534	83.55%	10.428%
13	7.628	2037	2049	2067	rBV	24468	45668	6.53%	0.815%
14	8.095	2183	2194	2235	rBV	210535	449074	64.19%	8.011%
15	8.853	2415	2430	2457	rBV	370210	609821	87.17%	10.879%
16	10.217	2841	2854	2875	rVB	103213	166193	23.76%	2.965%
17	11.249	3164	3175	3201	rBV	332264	520331	74.38%	9.283%
18	11.622	3279	3291	3315	rBV	274966	439776	62.86%	7.846%
19	16.483	4794	4803	4814	rBV2	11756	18117	2.59%	0.323%




Sum of corrected areas: 5605374

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026537.D
Acq On : 24 Jun 2022 01:06
Operator : SY/MD
Sample : VV0623WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK384

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

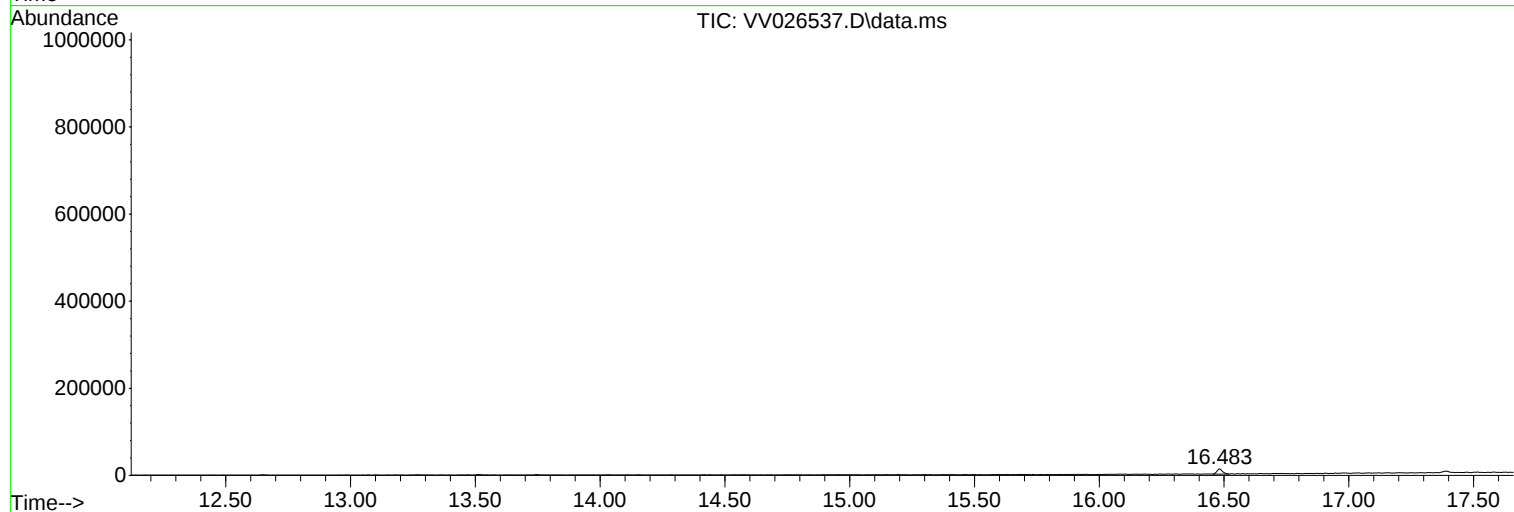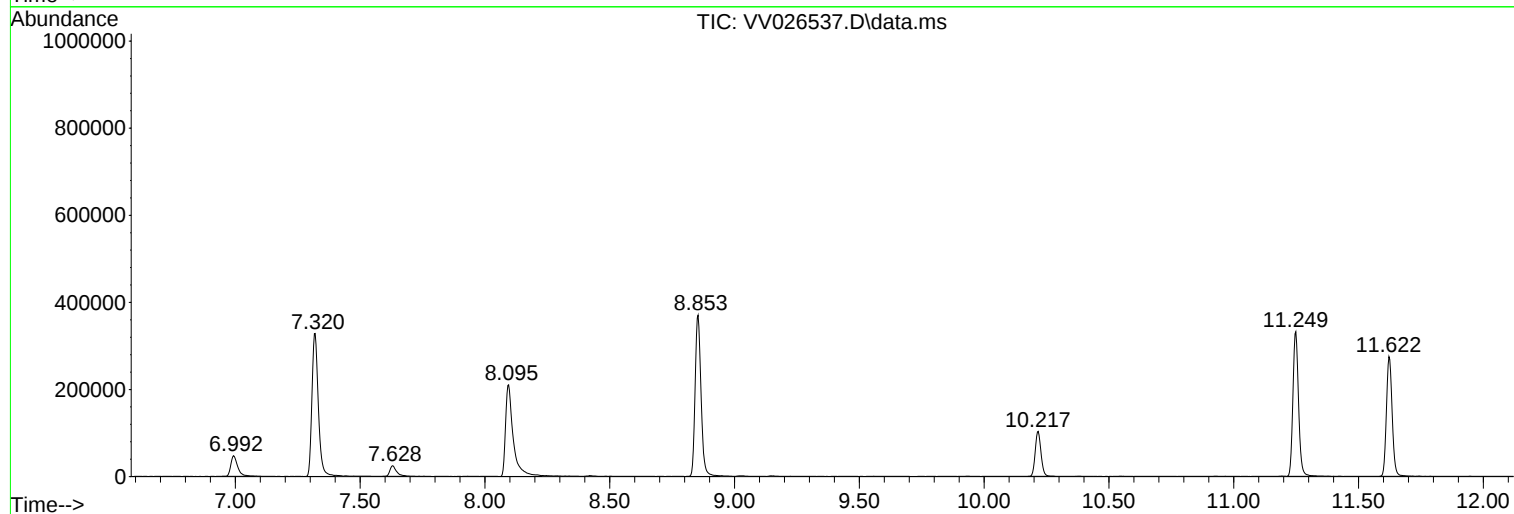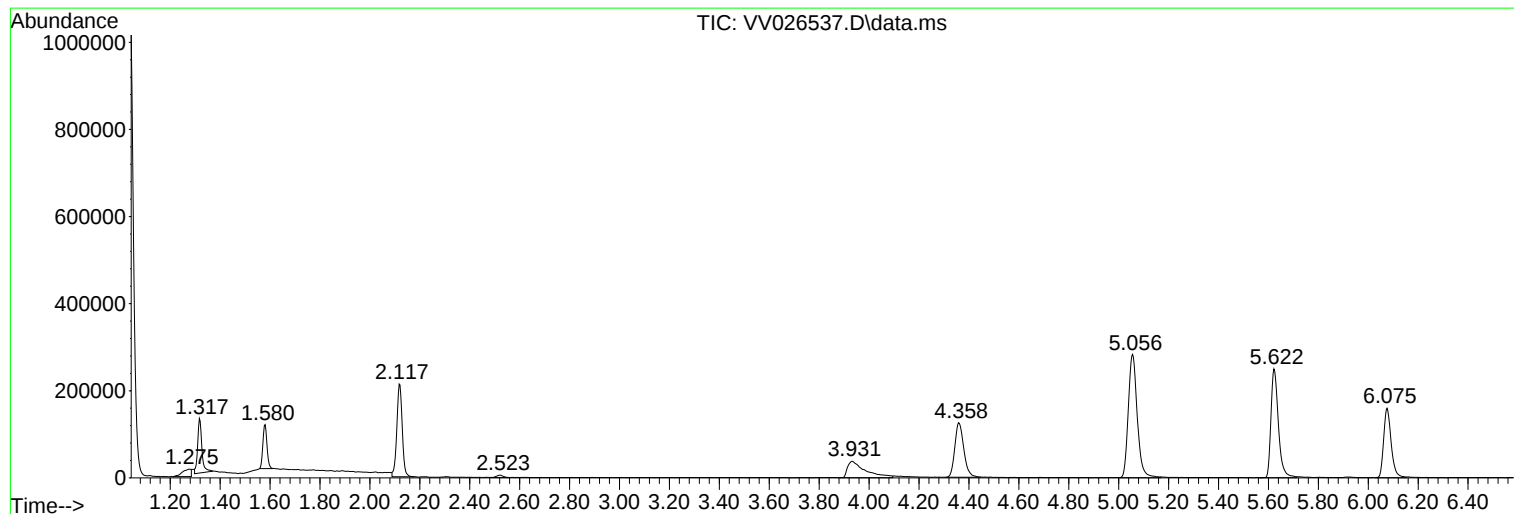

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026537.D
Acq On : 24 Jun 2022 01:06
Operator : SY/MD
Sample : VV0623WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK384

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026537.D
Acq On : 24 Jun 2022 01:06
Operator : SY/MD
Sample : VV0623WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK384

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc