


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026503.D
Acq On : 23 Jun 2022 09:57
Operator : SY/MD
Sample : BFB335
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB335

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jun 28 01:50:05 2022

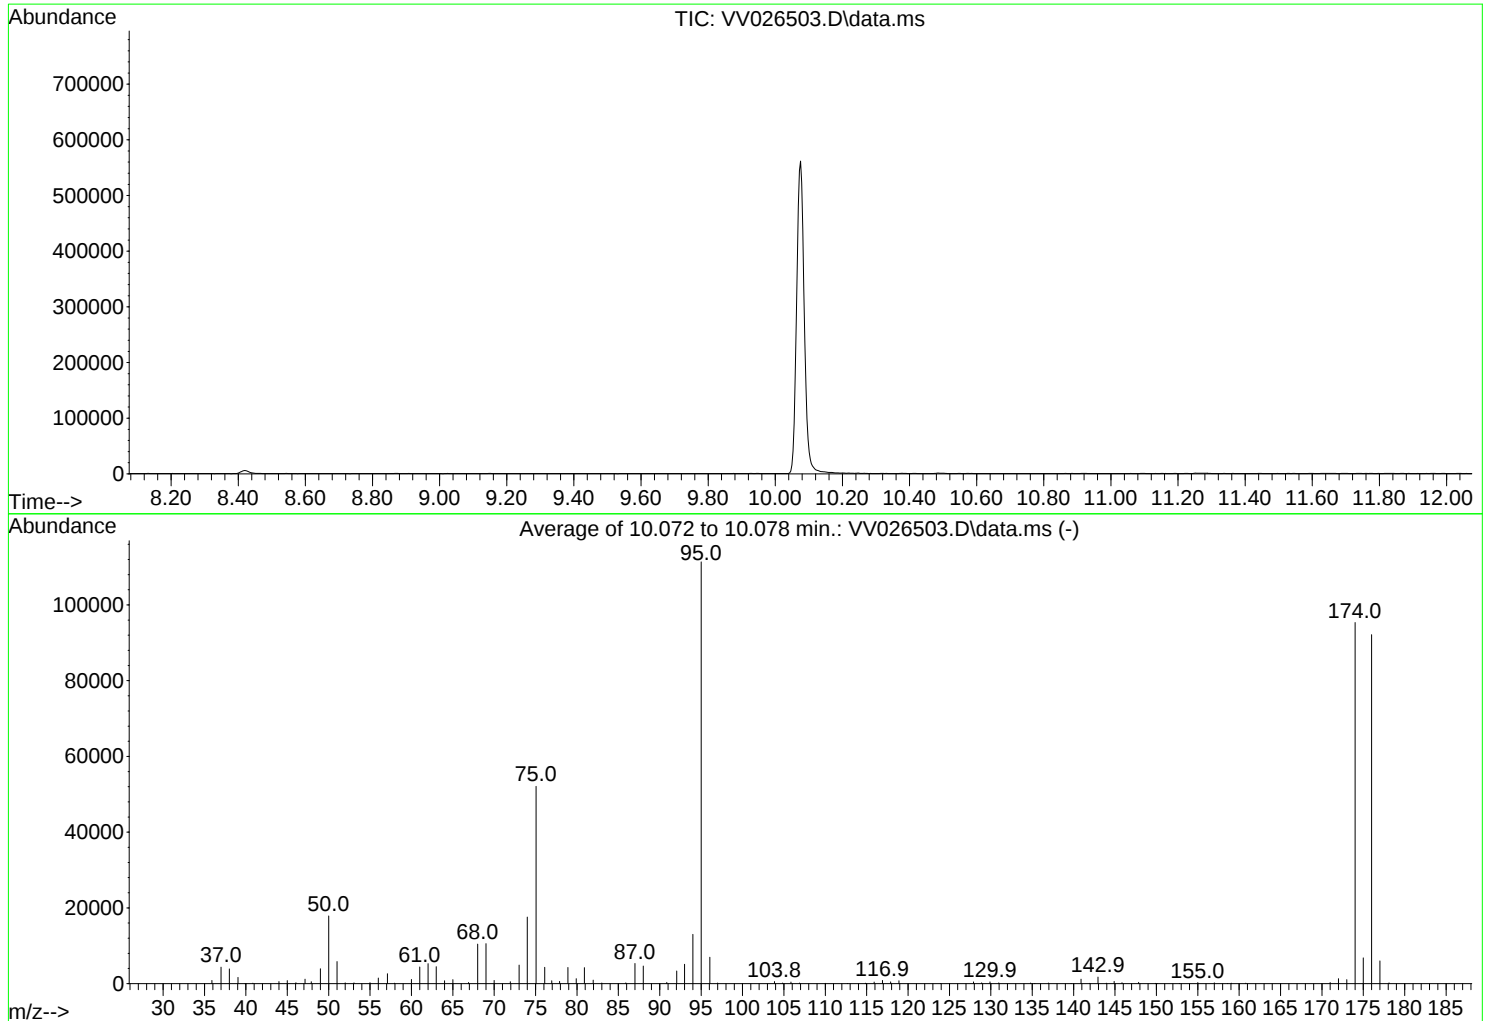

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	17864	PASS
75	95	30	80	46.8	52107	PASS
95	95	100	100	100.0	111376	PASS
96	95	5	9	6.3	6975	PASS
173	174	0.00	2	1.1	1078	PASS
174	95	50	120	85.6	95376	PASS
175	174	5	9	7.1	6804	PASS
176	174	95	105	96.6	92149	PASS
177	176	5	10	6.5	6010	PASS

m/z	Abundance
40.00	234.0
44.00	327.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	830.0
37.00	4534.0
38.00	4013.0
39.00	1719.0
39.90	241.0
40.80	122.0
44.00	932.0
45.00	802.0
46.10	280.0
47.10	1227.0
47.90	597.0
49.00	4052.0
50.00	18368.0
51.00	5983.0
52.00	224.0
53.10	199.0
55.00	288.0
56.00	1389.0
57.10	2605.0
58.00	160.0
60.00	1077.0
61.00	4474.0
62.00	5417.0
63.00	4422.0
64.00	814.0
65.00	1055.0
66.90	291.0
68.00	10655.0
69.00	10692.0
70.00	823.0
72.00	544.0
73.00	5030.0
74.00	17624.0
75.10	53112.0
76.10	4583.0
77.00	786.0
77.90	526.0
78.90	4296.0
79.90	1323.0
80.90	4311.0
82.00	927.0
83.00	151.0
85.90	208.0
87.00	5277.0
88.00	4738.0
90.90	329.0
92.00	3276.0
93.00	5141.0
94.00	13005.0
95.00	112152.0
96.00	7195.0
97.00	130.0
103.90	551.0
104.90	203.0
105.80	378.0
106.90	142.0
114.90	114.0
115.90	436.0
116.90	856.0
117.90	474.0
118.90	693.0
127.90	399.0
128.90	187.0
129.90	443.0
131.00	214.0
134.80	171.0
136.90	201.0
140.90	1191.0
141.90	155.0
142.90	1862.0
143.90	138.0
144.90	622.0
145.80	219.0
147.90	302.0
149.90	146.0
155.00	285.0
157.00	220.0
159.00	133.0
171.00	333.0
172.00	1290.0
173.00	1179.0
174.00	94776.0
175.00	6857.0
176.00	90176.0
177.00	6083.0
178.10	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	915.0
37.00	4514.0
38.00	4061.0
39.00	1716.0
39.90	266.0
40.90	147.0
44.00	897.0
45.00	826.0
46.10	252.0
47.20	1230.0
47.90	503.0
49.00	4035.0
50.00	18360.0
51.00	6084.0
52.00	220.0
53.10	238.0
55.00	246.0
56.00	1518.0
57.10	2758.0
57.90	160.0
60.00	1140.0
61.00	4430.0
62.00	5562.0
63.00	4639.0
64.00	790.0
65.00	1066.0
66.90	290.0
68.00	10810.0
69.00	10891.0
70.00	863.0
71.90	539.0
73.00	5083.0
74.00	18088.0
75.00	53592.0
76.10	4438.0
76.90	781.0
77.90	645.0
78.90	4443.0
79.90	1394.0
80.90	4419.0
81.90	981.0
83.00	159.0
85.90	213.0
87.00	5588.0
88.00	4804.0
90.80	332.0
92.10	3453.0
93.00	5274.0
94.00	13430.0
95.00	115352.0
96.00	7254.0
97.00	184.0
103.90	557.0
104.80	193.0
105.90	424.0
106.90	176.0
110.00	114.0
112.70	114.0
114.80	162.0
115.90	433.0
116.90	834.0
117.90	480.0
118.90	797.0
123.90	107.0
127.90	466.0
128.90	199.0
129.90	487.0
131.00	213.0
134.80	183.0
135.30	113.0
137.00	196.0
140.90	1241.0
142.00	156.0
143.00	1781.0
144.00	140.0
144.90	623.0
145.80	262.0
147.90	320.0
149.90	156.0
155.00	329.0
157.00	244.0
159.10	144.0
160.80	168.0
171.00	311.0
172.00	1348.0
173.00	1083.0
174.00	98504.0
175.00	6966.0
176.00	95528.0
177.00	6190.0
178.10	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	855.0
37.00	4035.0
38.00	3561.0
39.10	1542.0
39.90	262.0
40.80	120.0
44.00	861.0
45.00	804.0
46.00	208.0
47.20	1037.0
47.90	394.0
49.00	3706.0
50.00	16864.0
51.00	5433.0
52.00	242.0
53.00	249.0
55.00	210.0
56.00	1473.0
57.10	2511.0
57.90	125.0
60.00	1066.0
61.00	4227.0
62.00	4904.0
63.00	4421.0
64.00	729.0
65.00	1023.0
66.90	285.0
68.00	9826.0
69.00	10159.0
70.00	900.0
71.90	487.0
73.00	4589.0
74.00	16992.0
75.00	49616.0
76.10	3972.0
76.90	682.0
77.90	598.0
78.90	4056.0
79.90	1275.0
80.90	4011.0
81.90	944.0
83.00	153.0
85.90	213.0
87.00	5144.0
88.00	4421.0
90.80	336.0
92.10	3239.0
93.00	4933.0
94.00	12661.0
95.00	106624.0
96.10	6476.0
97.00	228.0
103.80	540.0
104.80	171.0
105.90	448.0
106.90	160.0
110.00	120.0
114.80	175.0
115.90	406.0
116.90	796.0
117.90	424.0
118.90	779.0
127.90	479.0
128.90	190.0
129.90	459.0
130.90	176.0
134.80	212.0
137.00	170.0
139.70	103.0
140.90	1170.0
143.00	1602.0
144.00	131.0
144.90	572.0
145.90	296.0
147.80	341.0
150.10	122.0
152.80	105.0
155.00	302.0
157.00	235.0
158.60	118.0
159.10	140.0
160.80	252.0
171.00	273.0
172.00	1297.0
173.00	971.0
174.00	92848.0
175.00	6588.0
176.00	90744.0
177.00	5757.0
178.10	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335