
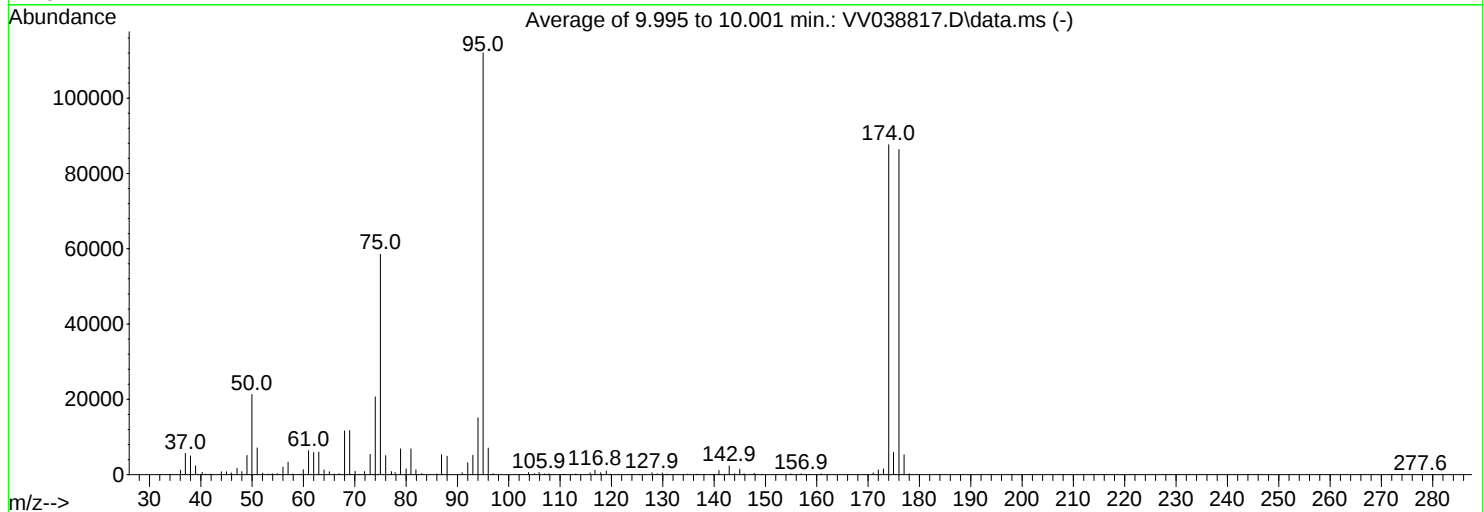


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV062325\
Data File : VV038817.D
Acq On : 23 Jun 2025 08:07
Operator : SY/MD
Sample : BFB238
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB238

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM061625.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jun 21 03:37:28 2025

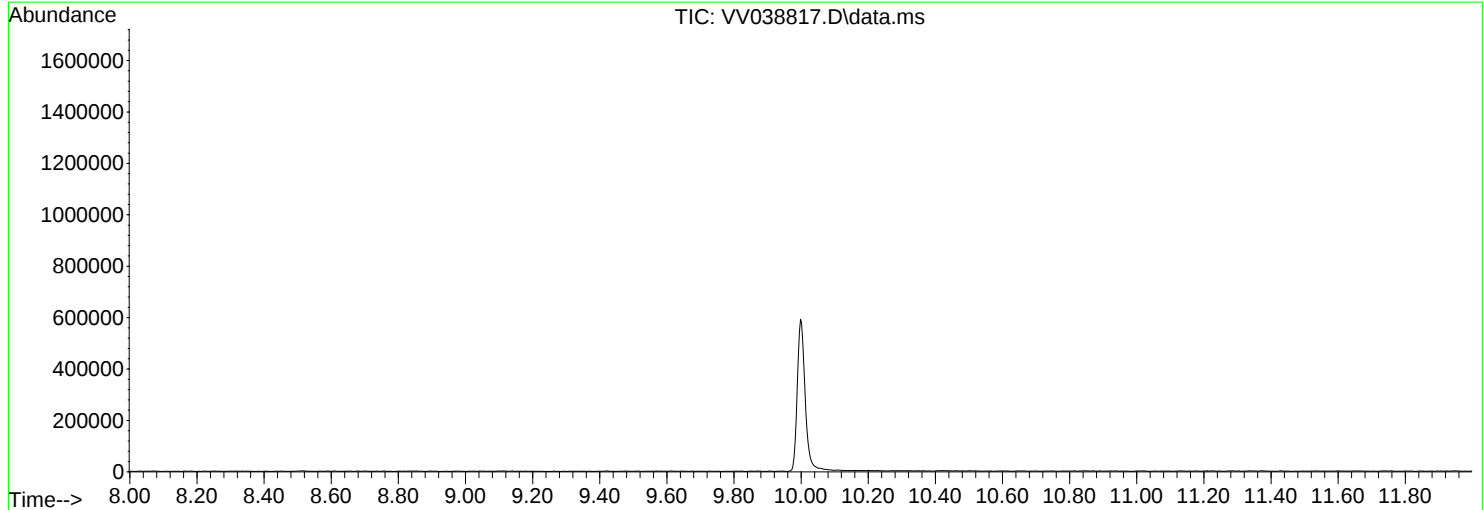

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2772

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	21295	PASS
75	95	30	80	52.2	58536	PASS
95	95	100	100	100.0	112037	PASS
96	95	5	9	6.3	7045	PASS
173	174	0.00	2	1.7	1520	PASS
174	95	50	120	78.2	87629	PASS
175	174	5	9	6.7	5892	PASS
176	174	95	101	98.6	86371	PASS
177	176	5	9	6.1	5294	PASS