

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062419\
 Data File : VV011733.D
 Acq On : 24 Jun 2019 16:26
 Operator : SY/MD
 Sample : K3462-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCN1

Quant Time: Jun 25 08:53:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 25 08:19:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	164201	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	152885	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	64584	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51257	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.57	69	40312	5.26	ug/L	-0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.20%
11) 1,1-Dichloroethene-d2	2.12	63	79146	3.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.40%
20) 2-Butanone-d5	3.94	46	160859	56.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.06%
24) Chloroform-d	4.40	84	104407	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.00%
26) 1,2-Dichloroethane-d4	5.08	65	62553	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.09	84	217945	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.12	67	67957	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.36	98	188785	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
43) trans-1,3-Dichloropropene-	7.66	79	20705	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.13	63	125211	58.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.28%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	48764	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	65053	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	4511	2.175 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062419\
Data File : VV011733.D
Acq On : 24 Jun 2019 16:26
Operator : SY/MD
Sample : K3462-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCN1

Quant Time: Jun 25 08:53:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 25 08:19:08 2019
Response via : Initial Calibration

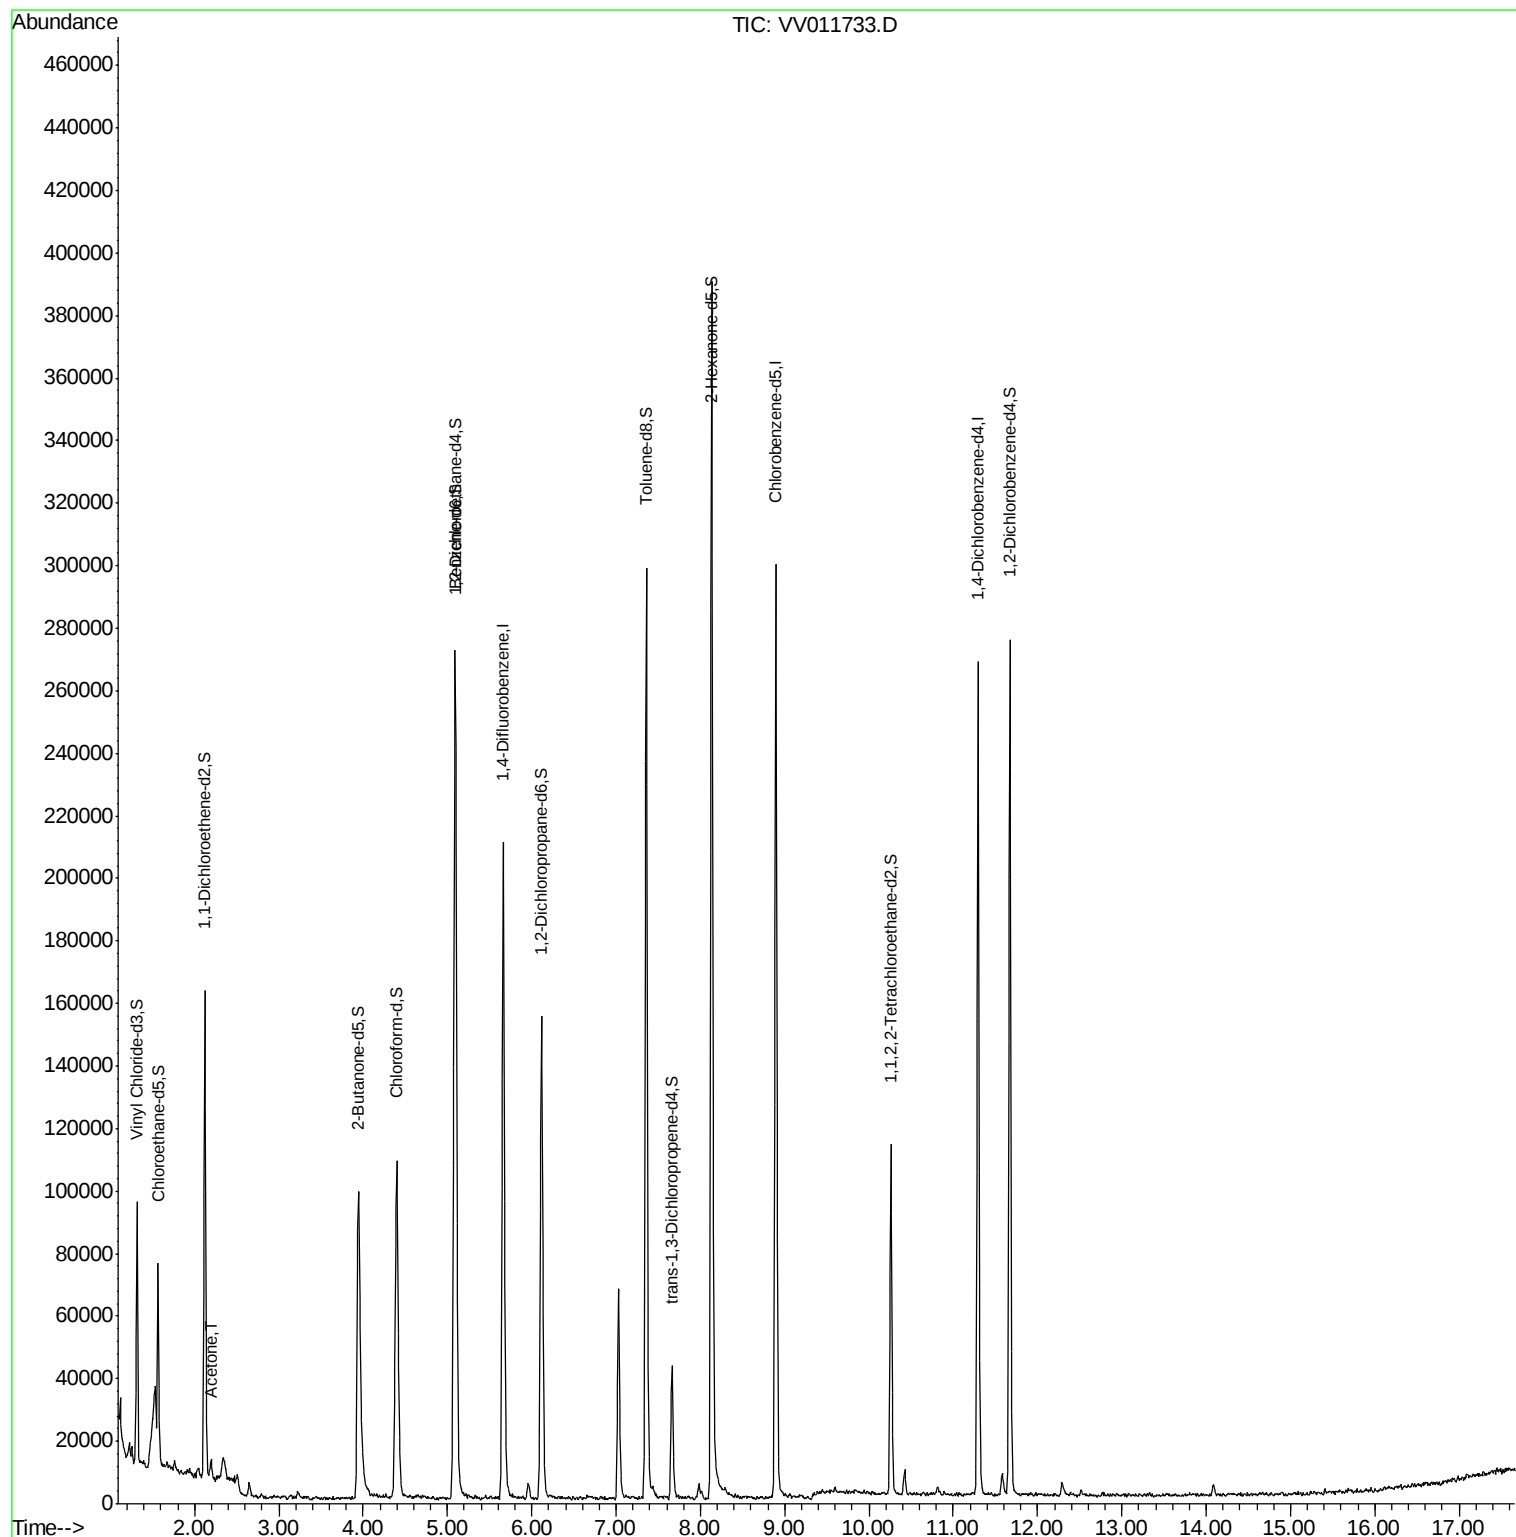

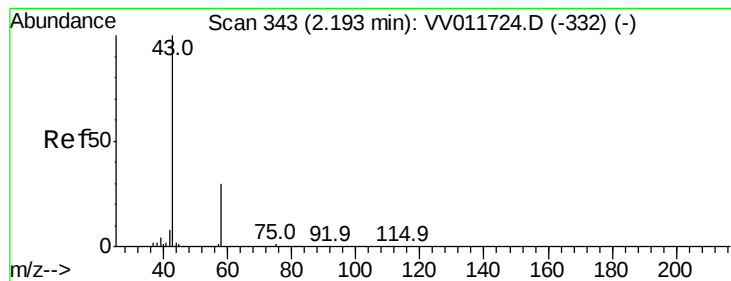

#13
 Acetone
 Concen: 2.175 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.00 min
 Lab File: VV011733.D
 Acq: 24 Jun 2019 16:26

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCN1

Tot Ion: 43 Resp: 4511
 Ion Ratio Lower Upper
 43 100
 58 35.8 0.0 56.6

