

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062419\
 Data File : VV011734.D
 Acq On : 24 Jun 2019 16:48
 Operator : SY/MD
 Sample : K3462-17
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCT9

Quant Time: Jun 25 08:55:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 25 08:19:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	162076	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	150731	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	63487	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51096	4.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.00%
7) Chloroethane-d5	1.57	69	38904	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.80%
11) 1,1-Dichloroethene-d2	2.12	63	78407	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	3.95	46	163714	57.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.54%
24) Chloroform-d	4.40	84	105939	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
26) 1,2-Dichloroethane-d4	5.08	65	62875	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
32) Benzene-d6	5.10	84	217562	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.12	67	68451	5.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.80%
41) Toluene-d8	7.36	98	188373	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	7.67	79	21063	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.14	63	123480	58.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.30%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	48788	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	65685	5.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	6349	3.102 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062419\
Data File : VV011734.D
Acq On : 24 Jun 2019 16:48
Operator : SY/MD
Sample : K3462-17
Misc : 25ML/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT9

Quant Time: Jun 25 08:55:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 25 08:19:08 2019
Response via : Initial Calibration

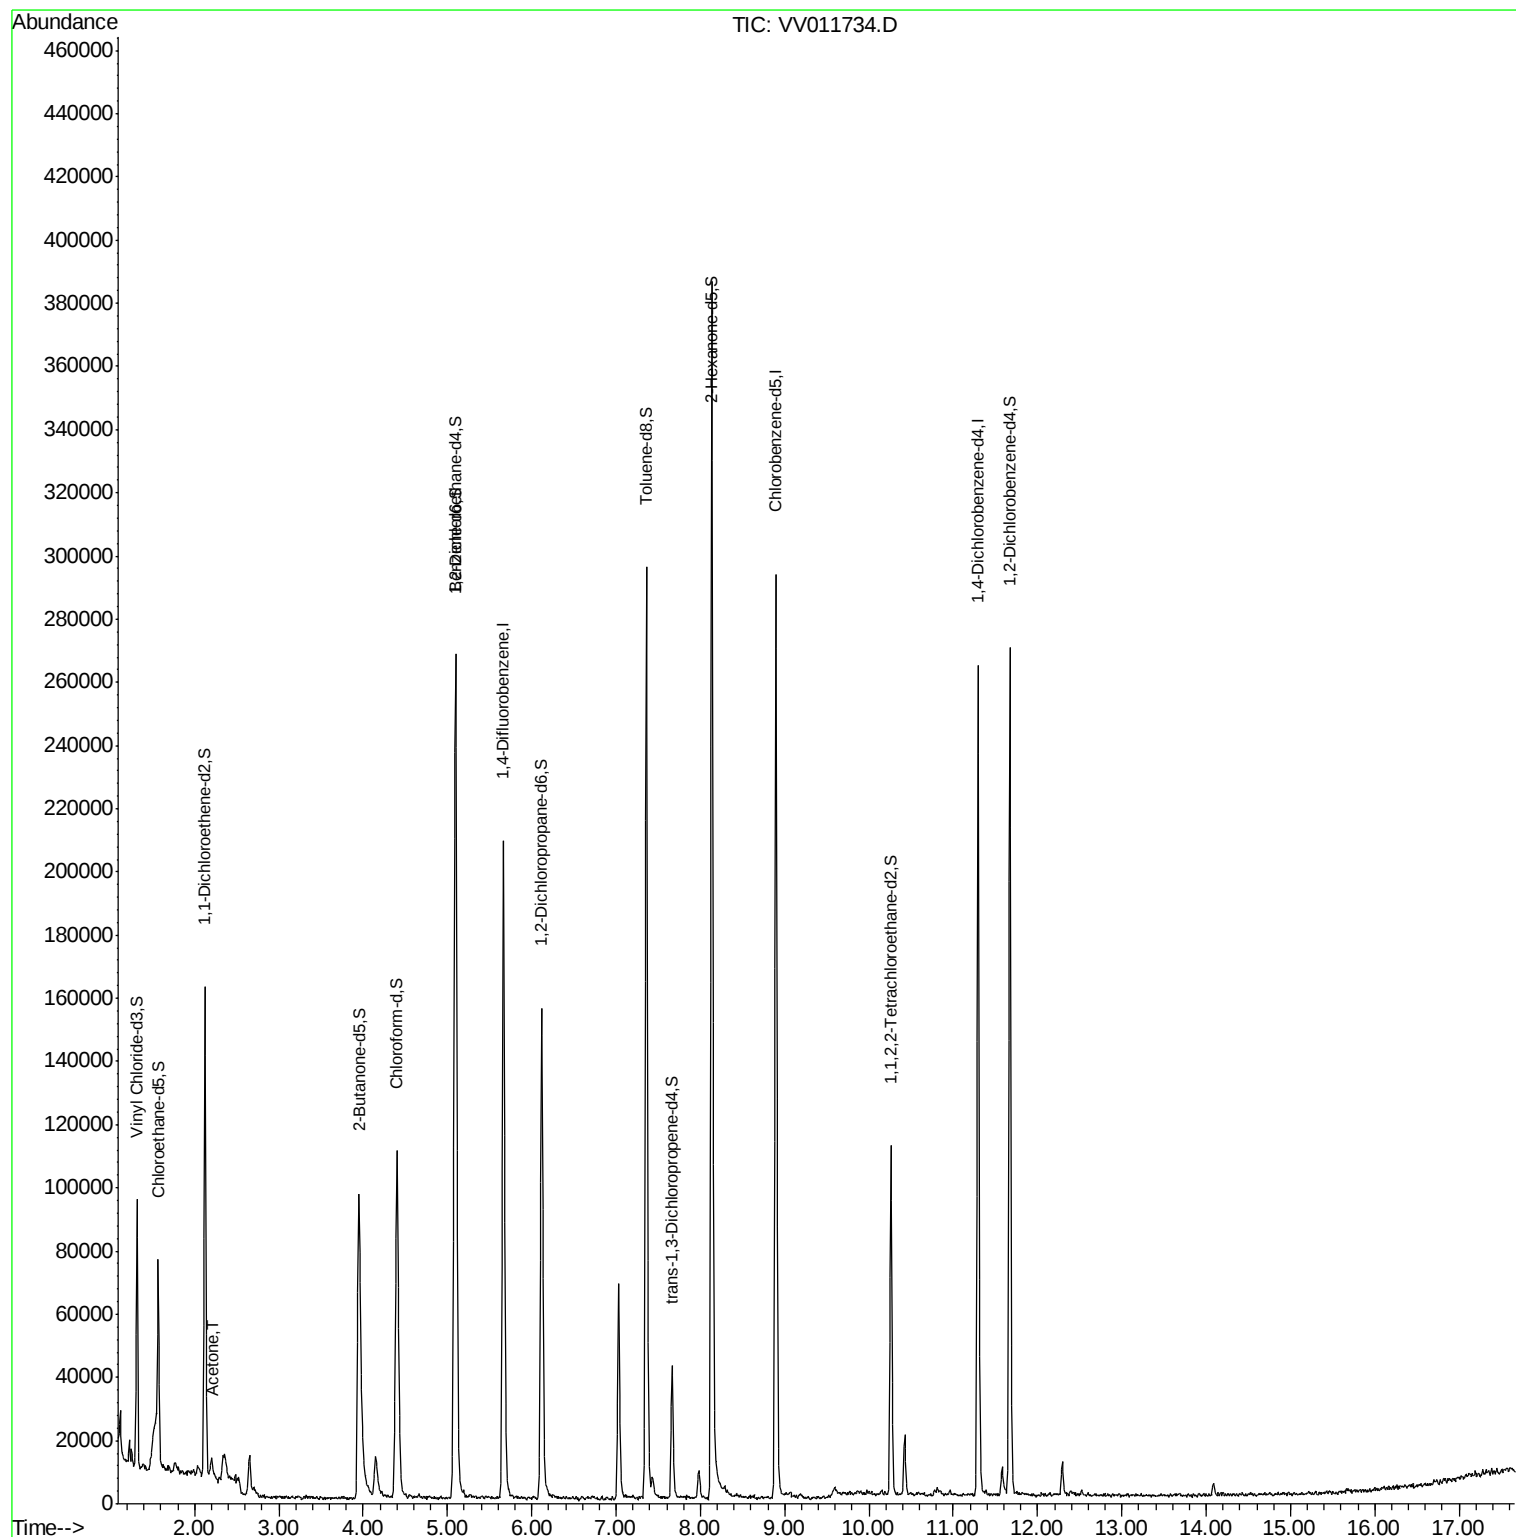

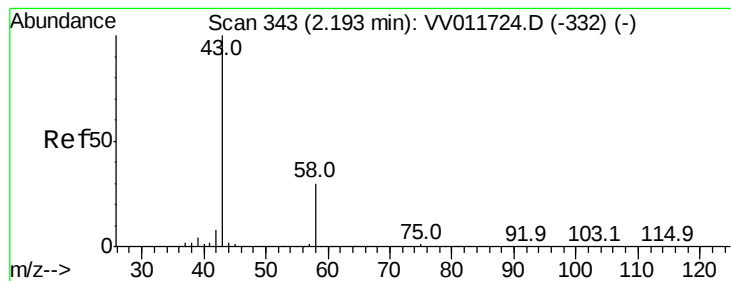

#13

Acetone

Concen: 3.102 ug/L

RT: 2.20 min Scan# 346

Delta R.T. 0.01 min

Lab File: VV011734.D

Acq: 24 Jun 2019 16:48

Instrument :
MSVOA_V
ClientSampleId :
BFCT9

Tot Ion: 43 Resp: 6349

Ion Ratio Lower Upper

43 100

58 31.1 0.0 56.6

