

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062419\
 Data File : VV011735.D
 Acq On : 24 Jun 2019 17:35
 Operator : SY/MD
 Sample : K3462-16
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCT3

Quant Time: Jun 25 08:57:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 25 08:19:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	160197	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	148463	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	62673	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	53033	4.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.80%
7) Chloroethane-d5	1.58	69	38454	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.80%
11) 1,1-Dichloroethene-d2	2.12	63	81695	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.95	46	175896	62.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.60%
24) Chloroform-d	4.40	84	110010	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.40%
26) 1,2-Dichloroethane-d4	5.08	65	66244	5.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.60%
32) Benzene-d6	5.10	84	227098	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.60%
36) 1,2-Dichloropropane-d6	6.12	67	70613	5.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.80%
41) Toluene-d8	7.36	98	198949	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
43) trans-1,3-Dichloropropene-	7.66	79	22587	5.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.40%
46) 2-Hexanone-d5	8.13	63	132668	63.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	126.86%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	52294	5.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	118.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	68055	5.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	6332	3.130 ug/L	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062419\
Data File : VV011735.D
Acq On : 24 Jun 2019 17:35
Operator : SY/MD
Sample : K3462-16
Misc : 25ML/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT3

Quant Time: Jun 25 08:57:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 25 08:19:08 2019
Response via : Initial Calibration

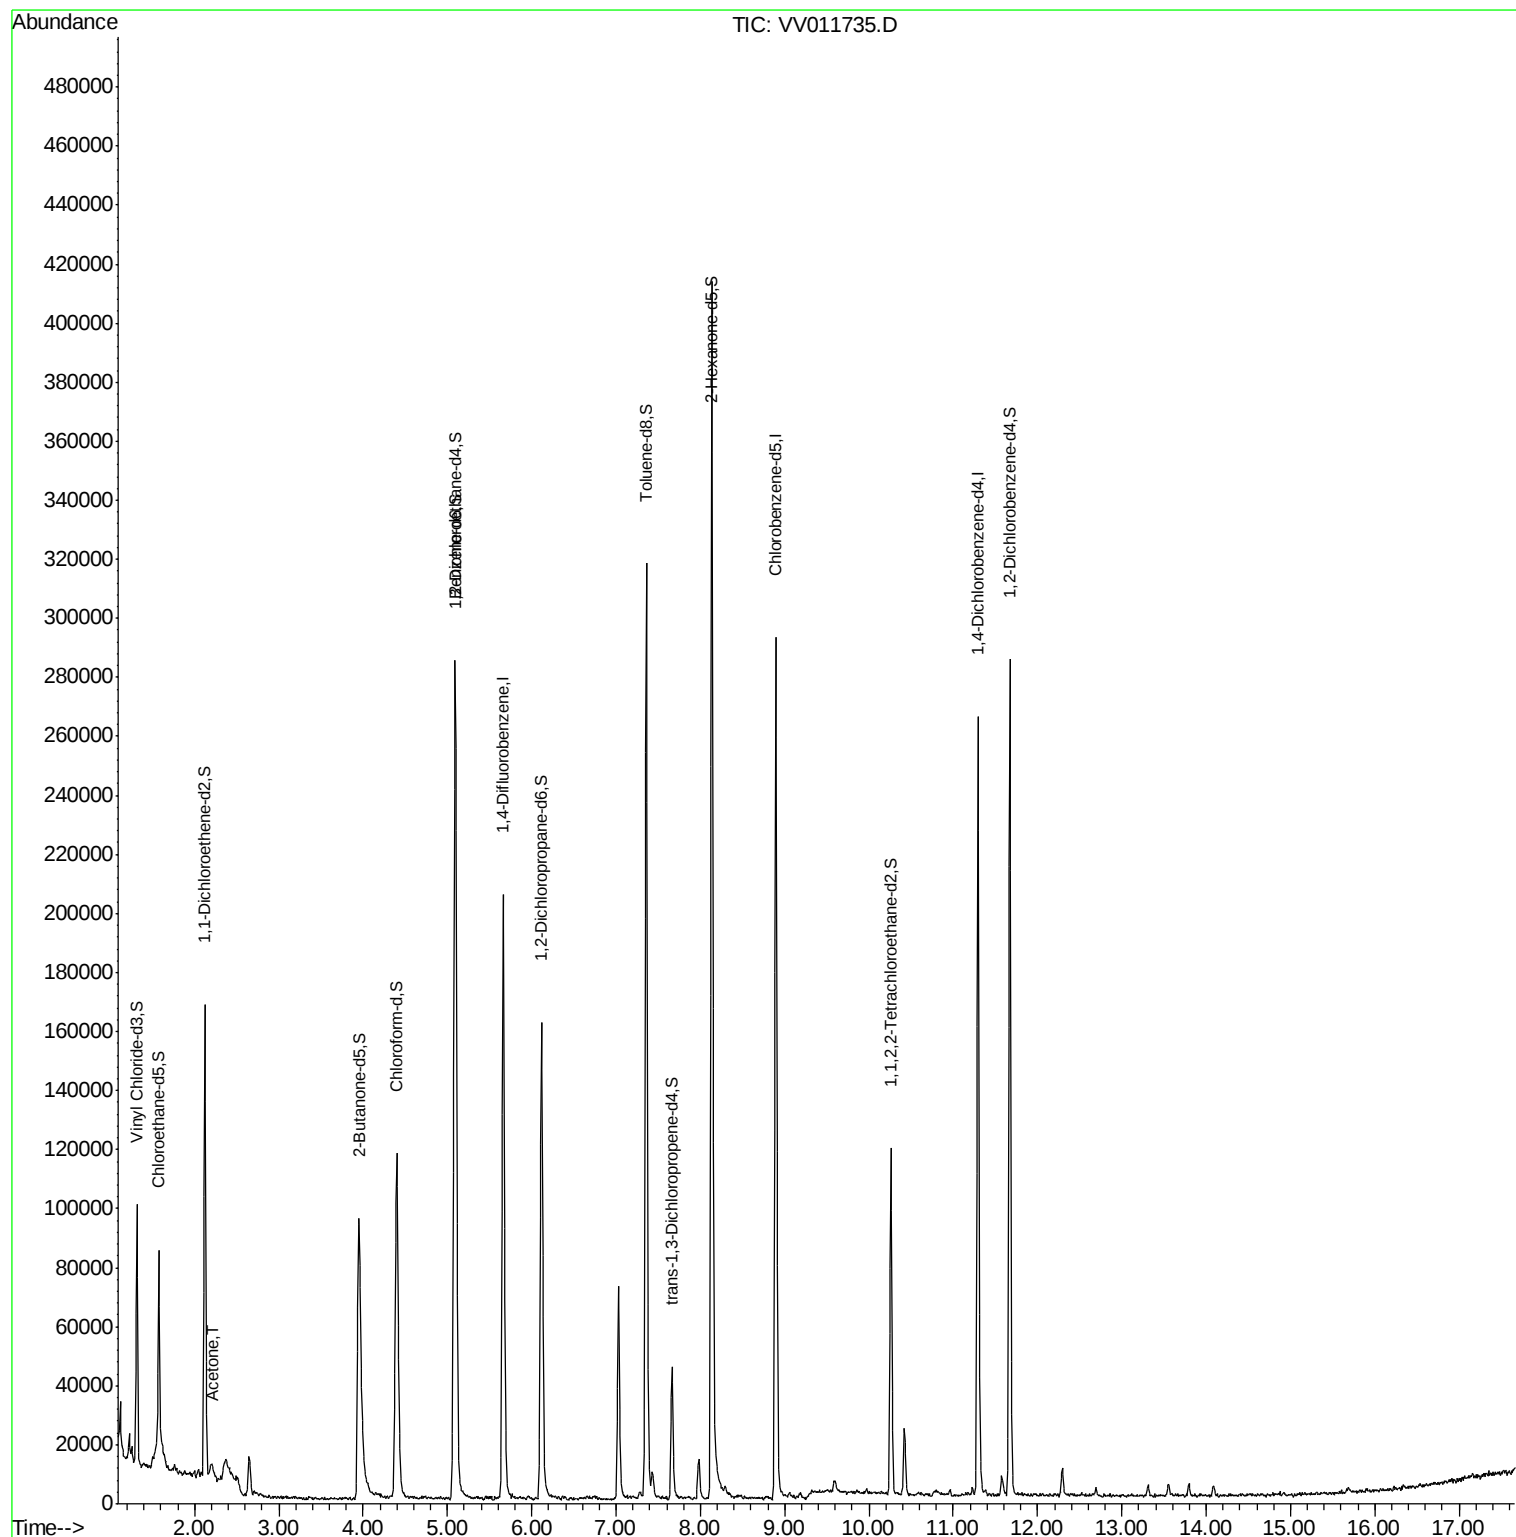

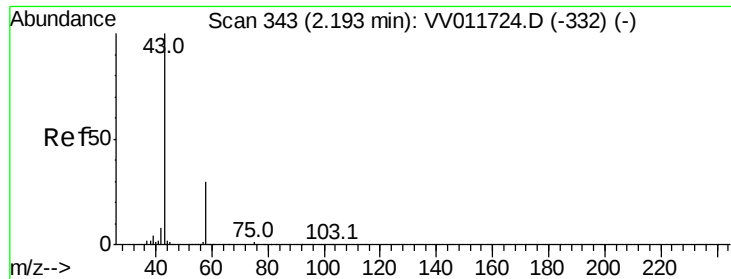

#13

Acetone

Concen: 3.130 ug/L

RT: 2.21 min Scan# 347

Delta R.T. 0.01 min

Lab File: VV011735.D

Acq: 24 Jun 2019 17:35

Instrument :
MSVOA_V
ClientSampleId :
BFCT3

Tot Ion: 43 Resp: 6332

Ion Ratio Lower Upper

43 100

58 13.0 0.0 56.6

