


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062419\
Data File : VV011723.D
Acq On : 24 Jun 2019 09:28
Operator : SY/MD
Sample : BFB55
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jun 25 08:19:08 2019

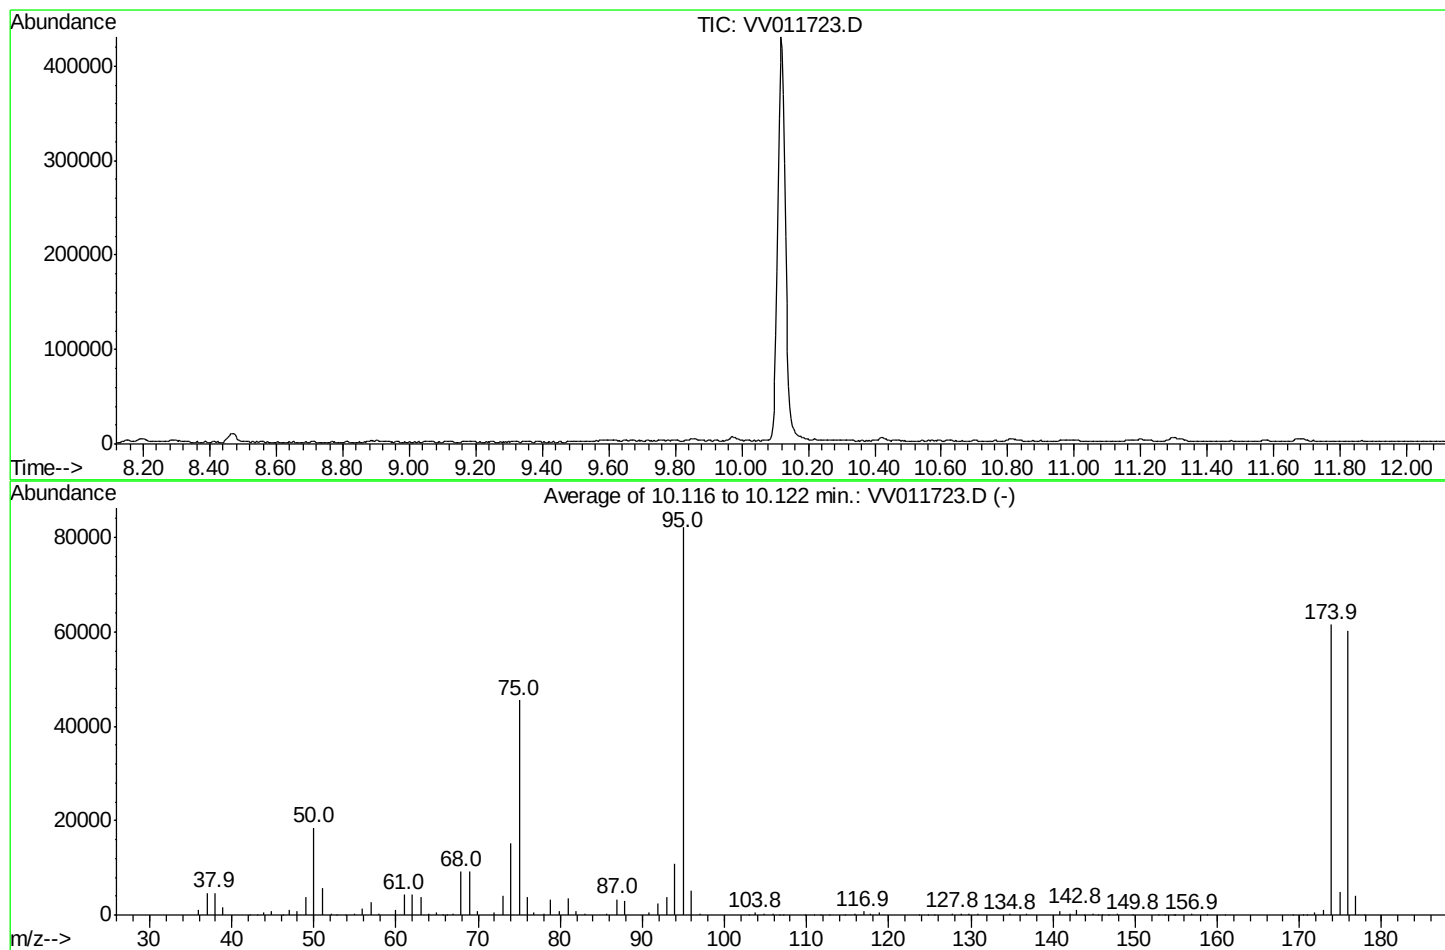

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	18514	PASS
75	95	30	80	55.4	45536	PASS
95	95	100	100	100.0	82181	PASS
96	95	5	9	6.4	5297	PASS
173	174	0.00	2	1.6	999	PASS
174	95	50	120	74.8	61512	PASS
175	174	5	9	8.1	5006	PASS
176	174	95	101	97.8	60138	PASS
177	176	5	9	6.7	4007	PASS

m/z	Abundance
35.90	1166.0
37.00	195.0
37.80	423.0
39.00	184.0
39.80	451.0
40.80	194.0
41.50	112.0
41.90	115.0
42.70	109.0
43.20	154.0
43.90	490.0
44.70	116.0
54.90	123.0
56.00	128.0
66.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	2168.0
37.00	4970.0
38.00	5049.0
39.00	1868.0
39.90	375.0
40.80	138.0
41.80	151.0
43.10	171.0
43.90	905.0
44.90	890.0
46.90	1022.0
47.90	690.0
49.00	3909.0
50.00	18336.0
51.00	5374.0
52.00	312.0
52.80	101.0
53.90	143.0
54.90	321.0
55.90	1601.0
56.90	2674.0
57.90	169.0
60.00	959.0
61.00	4304.0
62.00	4466.0
63.00	3800.0
63.90	345.0
64.90	508.0
65.70	110.0
66.20	105.0
67.00	331.0
68.00	8932.0
69.00	9260.0
70.00	791.0
71.90	495.0
73.00	4085.0
74.00	15319.0
75.00	44112.0
76.00	4033.0
76.80	455.0
77.90	326.0
78.80	3274.0
79.80	842.0
80.90	3518.0
81.80	736.0
83.00	146.0
85.60	171.0
87.00	3403.0
87.90	3060.0
90.80	473.0
91.90	2477.0
92.90	3719.0
94.00	10367.0
95.00	79064.0
96.00	5284.0
97.10	233.0
103.80	368.0
104.70	179.0
105.80	391.0
106.70	130.0
110.90	112.0
111.60	116.0
114.70	103.0
115.90	380.0
116.90	730.0
117.70	415.0
118.80	568.0
124.70	127.0
127.80	305.0
128.80	202.0
129.80	237.0
130.80	154.0
134.90	251.0
136.80	228.0
140.90	831.0
142.00	146.0
142.80	1101.0
143.80	106.0
144.80	161.0
145.50	122.0
147.80	353.0
149.80	111.0
152.90	144.0
153.60	108.0
154.70	120.0
157.00	169.0
158.80	136.0
160.90	117.0
169.20	142.0
170.50	106.0
171.80	541.0
173.00	912.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

173.90	57232.0
174.90	4823.0
175.90	57248.0
176.90	3780.0
177.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	2159.0
37.00	4953.0
38.00	5314.0
39.00	1775.0
39.90	410.0
40.90	154.0
41.80	127.0
42.10	115.0
42.80	147.0
43.10	157.0
43.90	1029.0
44.90	935.0
47.00	1025.0
48.00	699.0
49.00	3907.0
50.00	19176.0
51.00	5840.0
52.10	343.0
52.80	113.0
54.90	321.0
55.90	1650.0
56.90	2832.0
57.80	158.0
59.90	1055.0
61.00	4341.0
62.00	4605.0
63.00	4027.0
63.90	348.0
64.90	543.0
65.70	102.0
66.10	105.0
66.90	307.0
68.00	9543.0
69.00	9543.0
70.00	838.0
71.90	508.0
72.90	4058.0
74.00	15607.0
75.00	47232.0
76.00	4018.0
76.80	442.0
78.00	355.0
78.80	3334.0
79.90	946.0
80.90	3625.0
81.80	711.0
83.00	172.0
85.70	241.0
87.00	3402.0
87.90	3159.0
90.80	464.0
91.90	2491.0
92.90	3807.0
93.90	11132.0
95.00	84824.0
96.00	5489.0
97.10	238.0
103.80	424.0
104.80	213.0
105.90	381.0
106.70	100.0
107.10	102.0
109.80	101.0
110.80	125.0
111.70	121.0
112.80	123.0
114.70	128.0
115.90	369.0
116.90	798.0
117.70	391.0
118.80	581.0
123.70	118.0
125.50	108.0
127.80	322.0
128.80	187.0
129.80	301.0
130.90	169.0
134.80	249.0
136.80	252.0
140.80	903.0
142.00	157.0
142.80	1150.0
143.80	107.0
144.80	158.0
145.60	129.0
147.80	368.0
149.80	132.0
152.80	150.0
154.90	157.0
157.00	187.0
158.80	127.0
160.90	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

169.10	137.0
171.80	567.0
173.00	1000.0
173.90	63392.0
174.90	5210.0
175.90	61984.0
176.90	4134.0
177.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	2051.0
37.00	4611.0
37.90	4934.0
38.90	1611.0
39.90	444.0
40.90	156.0
42.70	129.0
43.20	152.0
43.90	1081.0
44.90	928.0
46.20	154.0
47.00	897.0
48.00	714.0
49.00	3675.0
50.00	18032.0
51.00	5763.0
52.20	313.0
52.80	124.0
54.90	316.0
55.90	1539.0
57.00	2692.0
57.90	137.0
59.90	1037.0
61.00	4218.0
62.00	4366.0
63.00	3881.0
63.90	386.0
64.90	502.0
66.90	265.0
67.90	9088.0
69.00	8907.0
69.90	765.0
71.80	528.0
72.90	3921.0
74.00	14684.0
75.00	45264.0
76.00	3680.0
76.80	430.0
78.00	374.0
78.80	3106.0
79.90	937.0
80.90	3375.0
81.90	698.0
82.90	158.0
85.70	242.0
86.90	3169.0
87.90	3017.0
90.90	426.0
91.90	2466.0
92.90	3677.0
93.90	10829.0
95.00	82656.0
96.00	5119.0
97.10	265.0
102.90	106.0
103.80	463.0
104.90	239.0
105.90	372.0
110.80	126.0
111.70	107.0
112.80	139.0
114.70	138.0
115.90	358.0
116.90	780.0
117.80	339.0
118.80	582.0
123.70	113.0
125.50	118.0
127.80	297.0
128.80	166.0
129.70	384.0
130.80	175.0
134.70	205.0
136.70	262.0
140.80	906.0
142.00	150.0
142.80	1083.0
143.70	103.0
144.80	153.0
145.90	175.0
146.70	112.0
147.80	310.0
149.70	128.0
152.80	143.0
154.90	176.0
156.90	219.0
158.80	143.0
160.90	130.0
169.10	113.0
170.90	112.0
171.80	574.0
173.00	1085.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

173.90	63912.0
174.90	4987.0
175.90	61184.0
176.90	4109.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55