
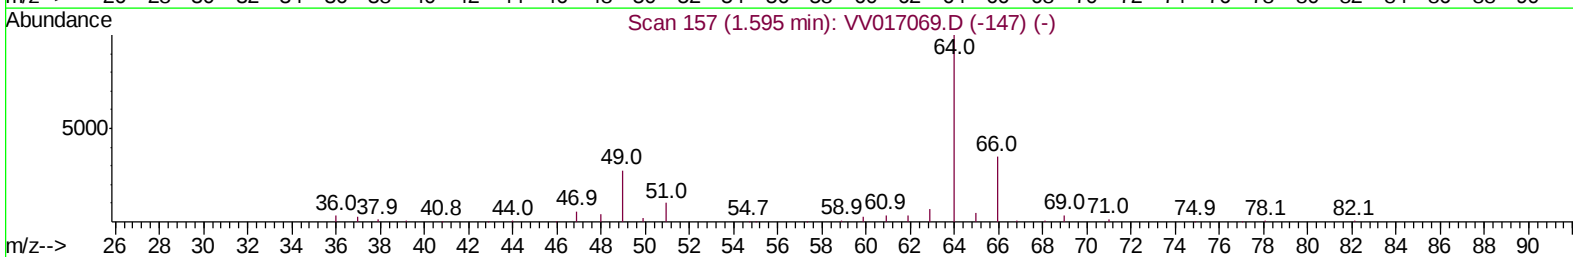
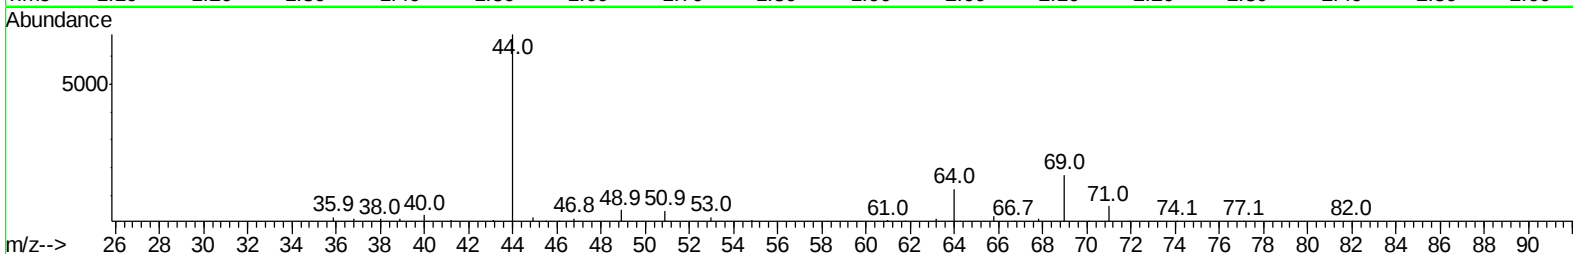


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062420\
Data File : VV017080.D
Acq On : 24 Jun 2020 18:41
Operator : SY/MD
Sample : L3105-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jun 25 01:20:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 01:16:55 2020
Response via : Initial Calibration

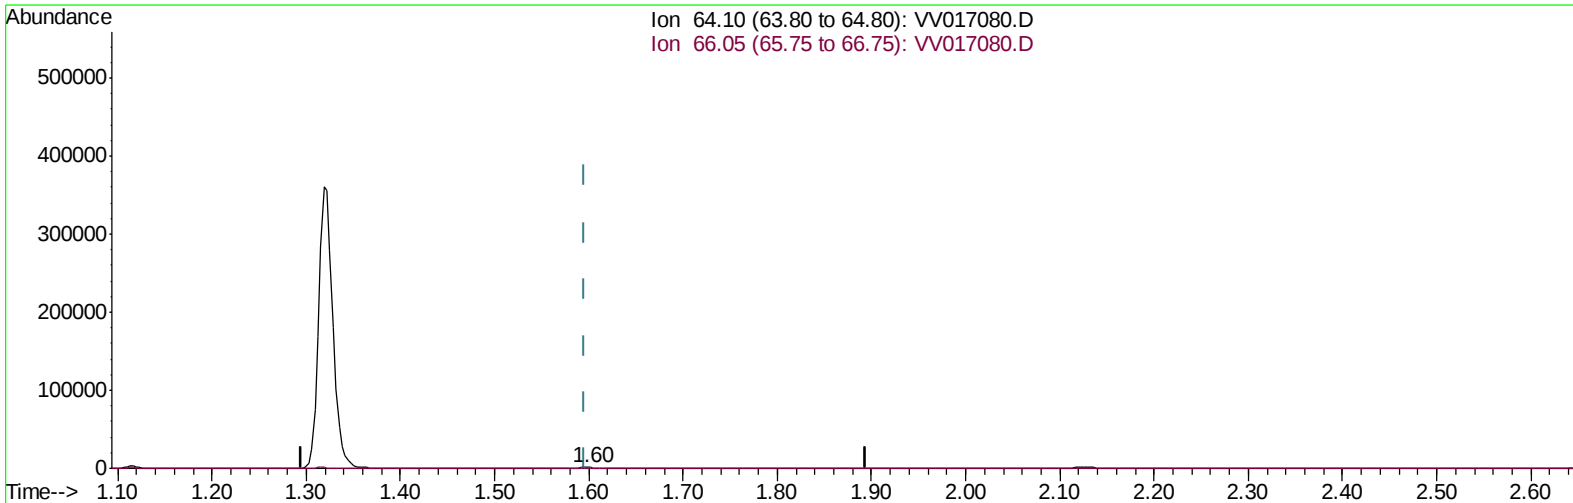

TIC: VV017080.D

(8) Chloroethane (T)

1.598min (+0.003) 0.24ug/L m

response 1526

Ion	Exp%	Act%
64.10	100	100
66.05	32.60	23.26
0.00	0.00	0.00
0.00	0.00	0.00