
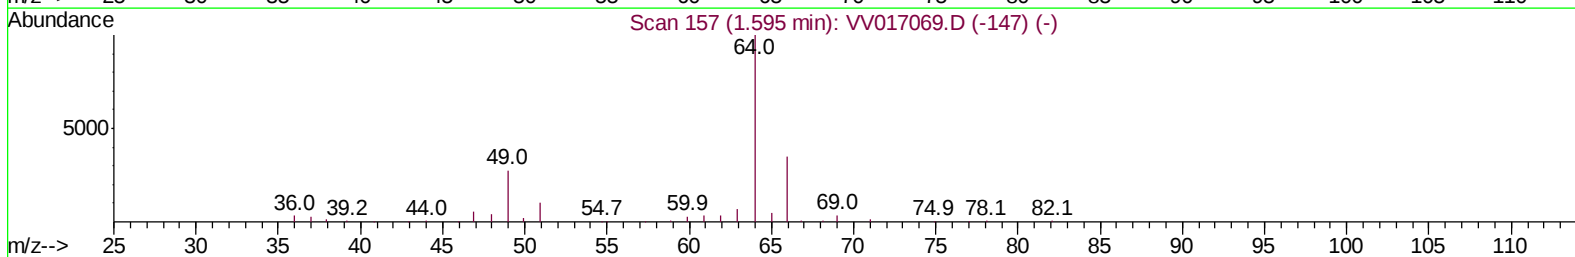
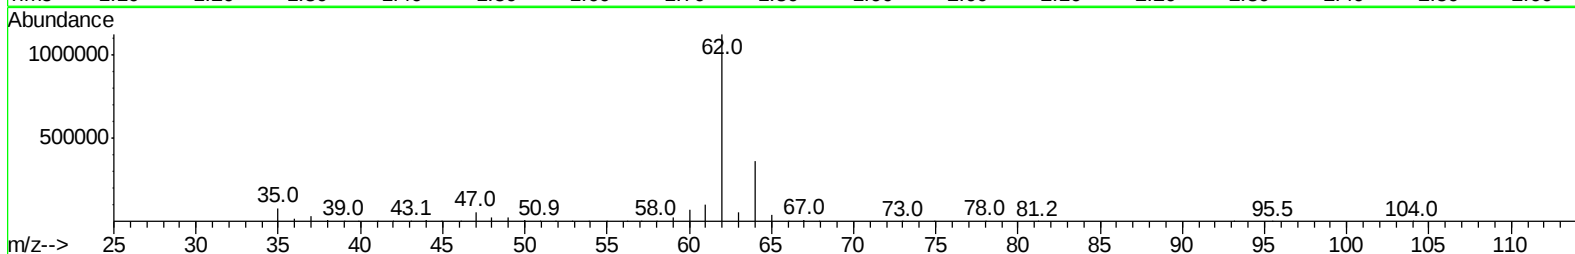


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062420\
Data File : VV017081.D
Acq On : 24 Jun 2020 19:05
Operator : SY/MD
Sample : L3105-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 25 01:21:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 01:16:55 2020
Response via : Initial Calibration

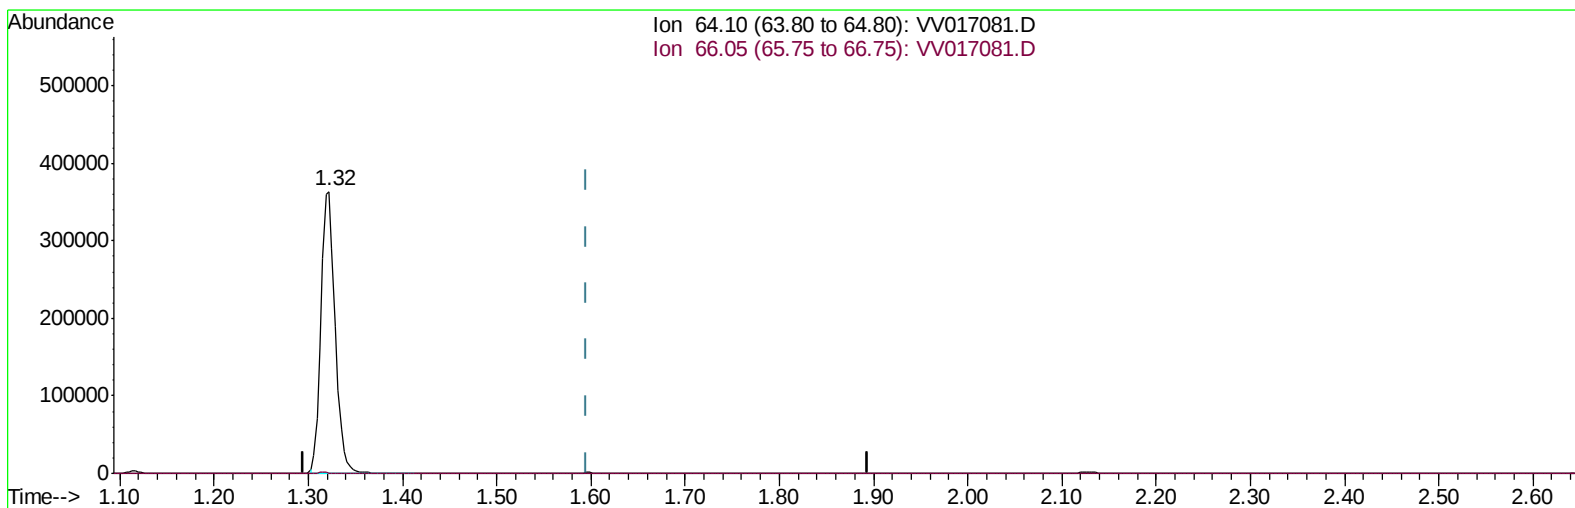

TIC: VV017081.D

(8) Chloroethane (T)

1.322min (-0.273) 59.26ug/L

response 379130

Ion	Exp%	Act%
64.10	100	100
66.05	32.60	0.21#
0.00	0.00	0.00
0.00	0.00	0.00