

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062420\
 Data File : VV017073.D
 Acq On : 24 Jun 2020 15:53
 Operator : SY/MD
 Sample : L3093-05DL 4X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTN4DL

Quant Time: Jun 25 01:57:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 25 01:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	173809	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	169144	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	79107	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	40278	3.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.20%
7) Chloroethane-d5	1.58	69	33866	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.13	63	63527	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	3.93	46	119898	45.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.20%
24) Chloroform-d	4.38	84	102865	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
26) 1,2-Dichloroethane-d4	5.06	65	55587	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
32) Benzene-d6	5.08	84	198090	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.10	67	57294	4.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.20%
41) Toluene-d8	7.34	98	176368	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
45) trans-1,3-Dichloropropene-	7.64	79	23204	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
48) 2-Hexanone-d5	8.11	63	89071	42.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.46%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	42856	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	70230	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
5) Vinyl chloride	1.32	62	54746	4.800 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062420\
Data File : VV017073.D
Acq On : 24 Jun 2020 15:53
Operator : SY/MD
Sample : L3093-05DL 4X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTN4DL

Quant Time: Jun 25 01:57:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 01:16:55 2020
Response via : Initial Calibration

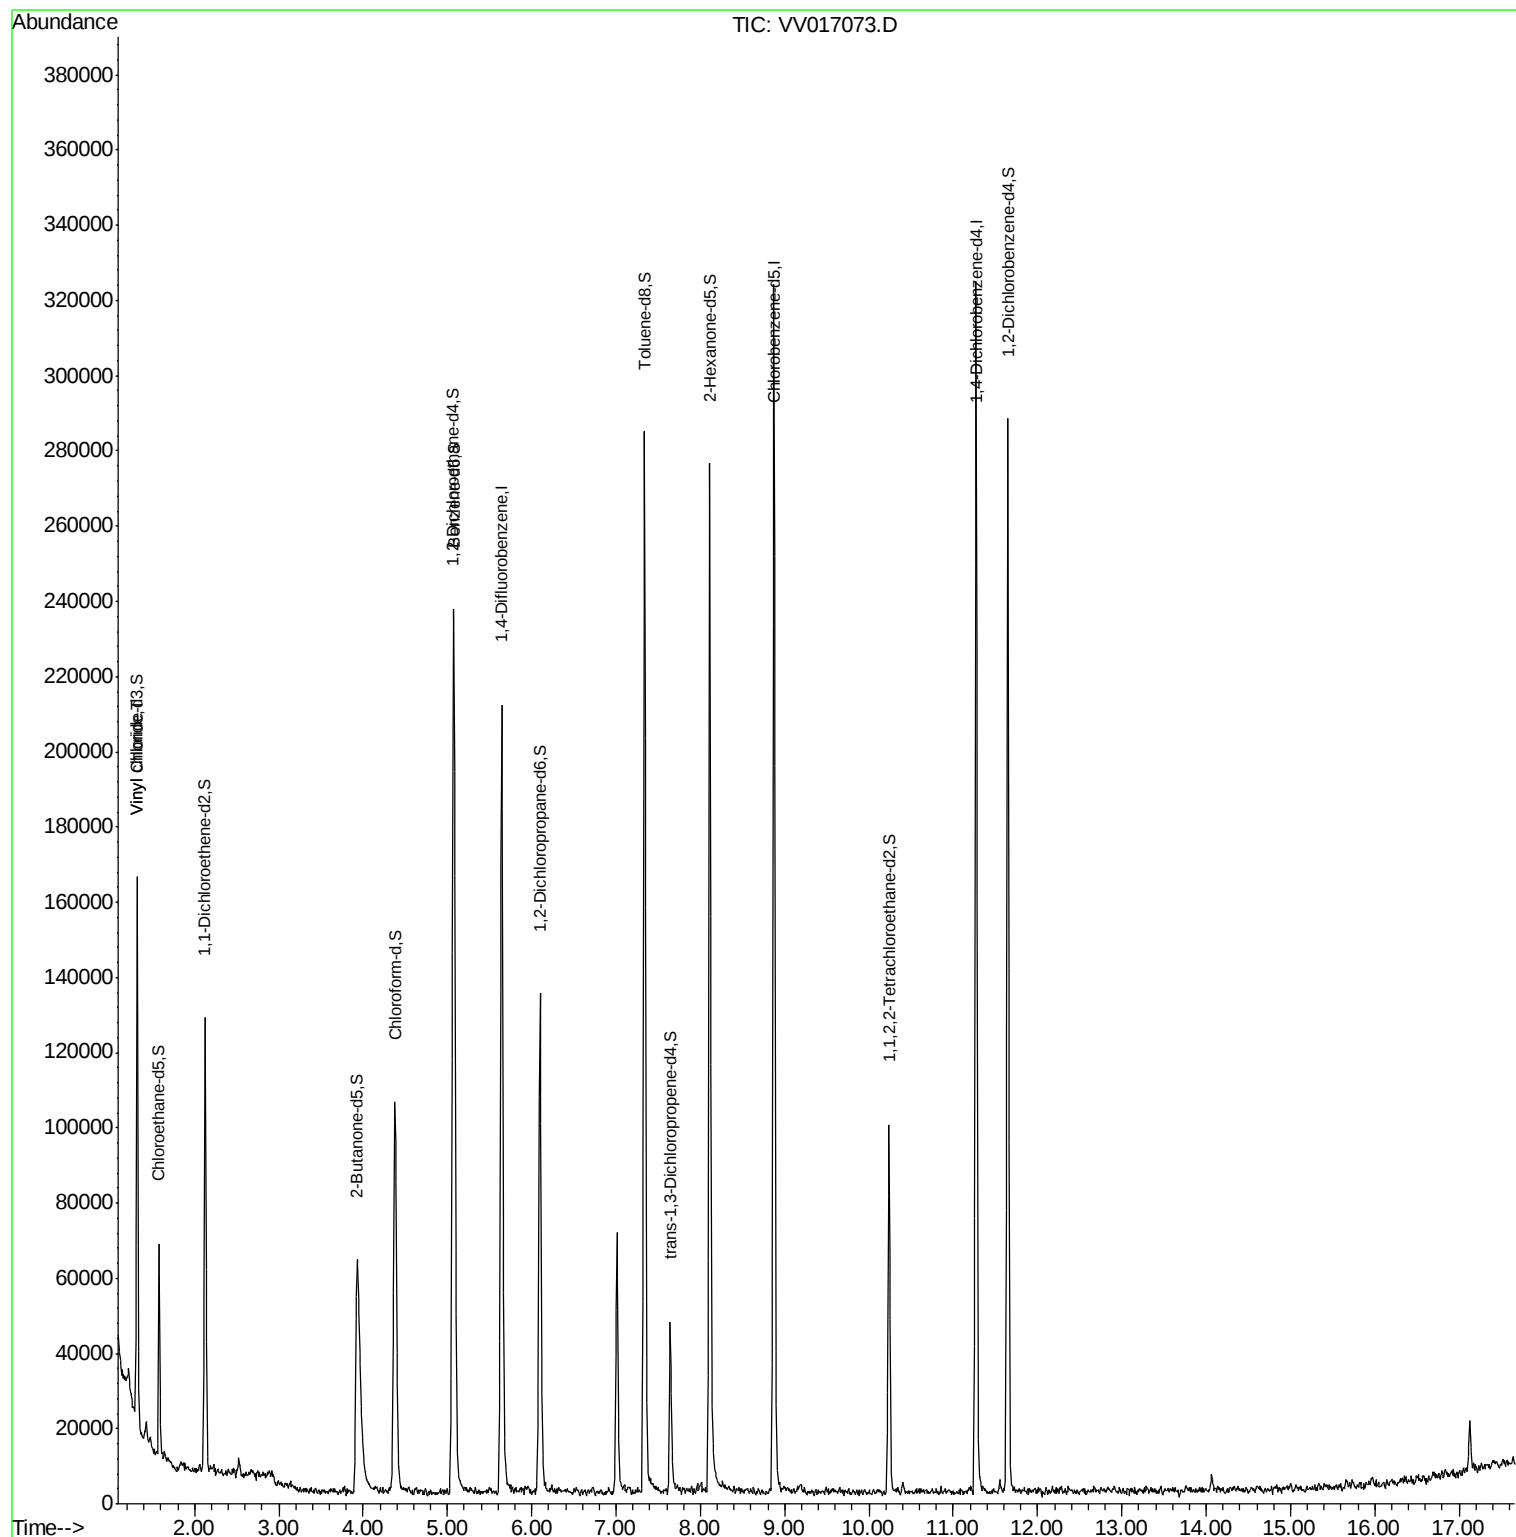

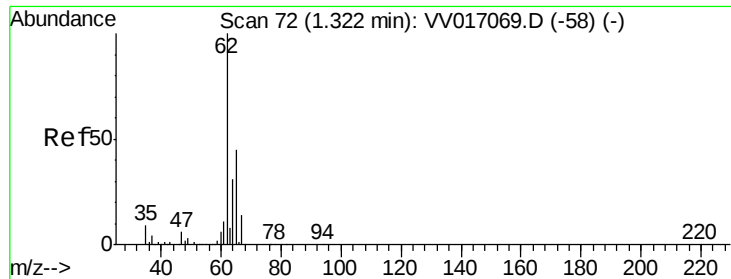

#5
 Vinyl chloride
 Concen: 4.800 ug/L
 RT: 1.32 min Scan# 72
 Delta R.T. -0.00 min
 Lab File: VV017073.D
 Acq: 24 Jun 2020 15:53

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTN4DL

Tot Ion: 62 Resp: 54746
 Ion Ratio Lower Upper
 62 100
 64 31.0 22.5 41.7

