

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062420\
 Data File : VV017116.D
 Acq On : 25 Jun 2020 09:52
 Operator : SY/MD
 Sample : L3102-20
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9L72

Quant Time: Jun 25 12:01:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 25 11:33:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	181417	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	173952	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	80636	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	37777	3.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.40%
7) Chloroethane-d5	1.58	69	31129	3.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.60%
11) 1,1-Dichloroethene-d2	2.13	63	58759	2.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.80%#
20) 2-Butanone-d5	3.93	46	116444	41.96	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.92%
24) Chloroform-d	4.38	84	99559	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.40%
26) 1,2-Dichloroethane-d4	5.06	65	54138	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.60%
32) Benzene-d6	5.08	84	187335	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.00%
36) 1,2-Dichloropropane-d6	6.10	67	57109	4.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.60%
41) Toluene-d8	7.34	98	167794	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
45) trans-1,3-Dichloropropene-	7.65	79	20442	3.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.60%
48) 2-Hexanone-d5	8.11	63	82934	38.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.36%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	40242	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	68575	4.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	5067	3.612 ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062420\
Data File : VV017116.D
Acq On : 25 Jun 2020 09:52
Operator : SY/MD
Sample : L3102-20
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9L72

Quant Time: Jun 25 12:01:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 11:33:08 2020
Response via : Initial Calibration

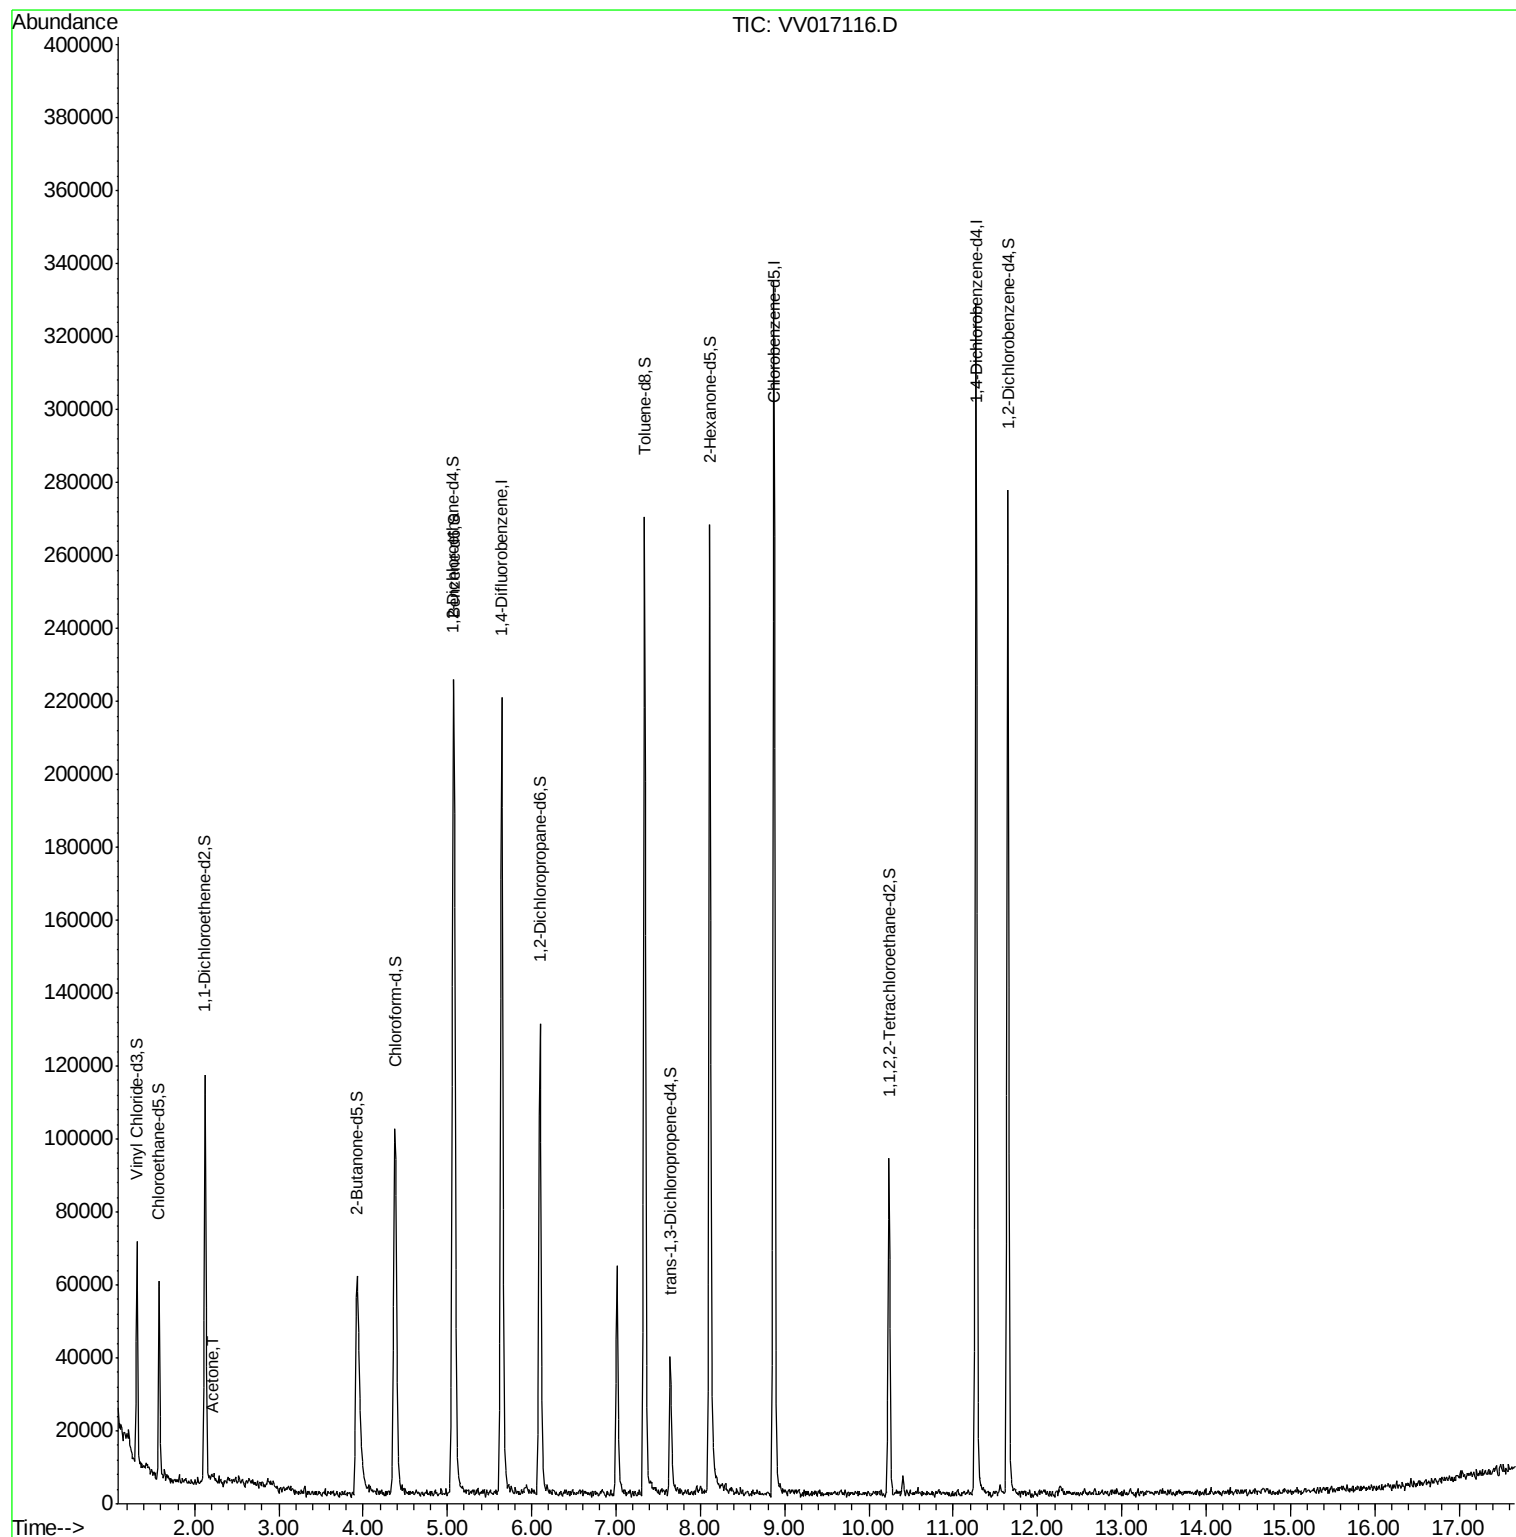

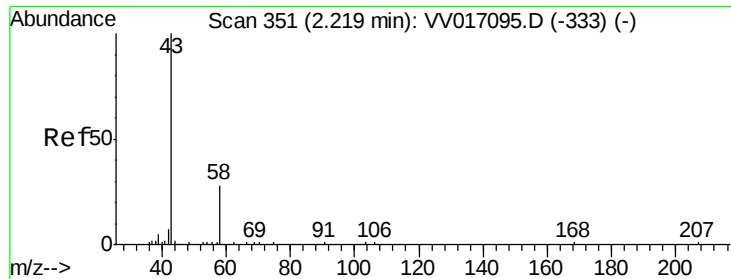

#13

Acetone

Concen: 3.612 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV017116.D

Acq: 25 Jun 2020 09:52

Instrument :

MSVOA_V

ClientSampleId :

F9L72

Tot Ion: 43 Resp: 5067

Ion Ratio Lower Upper

43 100

58 19.0 0.0 58.4

