


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062420\
 Data File : VV017068.D
 Acq On : 24 Jun 2020 13:38
 Operator : SY/MD
 Sample : BFB42
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 25 05:27:24 2020

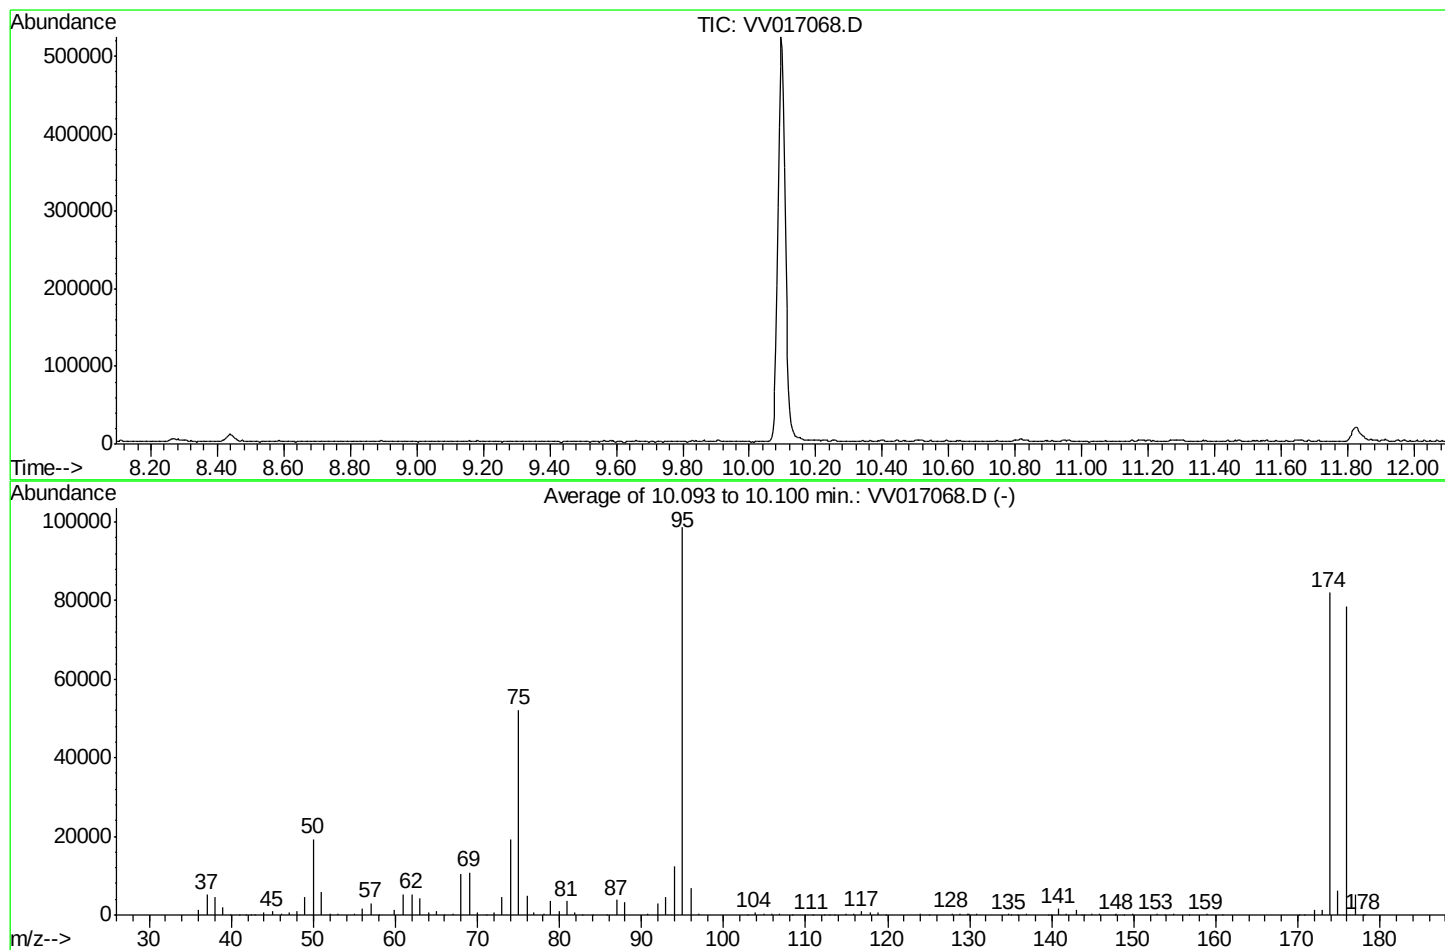

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	19338	PASS
75	95	30	80	52.8	52120	PASS
95	95	100	100	100.0	98642	PASS
96	95	5	9	7.0	6913	PASS
173	174	0.00	2	1.7	1382	PASS
174	95	50	120	83.2	82072	PASS
175	174	5	9	7.6	6252	PASS
176	174	95	101	95.6	78442	PASS
177	176	5	9	6.6	5158	PASS

m/z	Abundance
35.20	101.0
36.00	1346.0
37.00	5137.0
38.00	4691.0
39.00	2180.0
40.00	424.0
41.20	179.0
41.80	176.0
42.90	181.0
43.90	1000.0
45.00	918.0
46.10	285.0
47.00	828.0
48.00	930.0
49.00	4178.0
50.00	19264.0
51.00	5645.0
52.00	348.0
53.00	312.0
55.10	369.0
56.00	1845.0
57.00	2740.0
58.00	148.0
59.90	1157.0
61.00	5064.0
62.00	5335.0
63.00	4065.0
64.00	635.0
65.00	1001.0
66.00	250.0
67.00	500.0
68.00	10148.0
69.00	10243.0
70.00	760.0
72.00	548.0
73.00	4490.0
74.00	18776.0
75.00	50008.0
76.00	5028.0
76.90	594.0
78.10	552.0
78.90	3198.0
80.00	1164.0
80.90	3474.0
81.90	731.0
83.00	140.0
84.10	151.0
87.00	3829.0
87.90	3384.0
90.80	429.0
92.00	2848.0
93.00	4154.0
94.00	12050.0
95.00	95496.0
96.00	6712.0
97.00	236.0
103.90	594.0
105.00	178.0
105.90	514.0
106.90	214.0
112.20	127.0
112.80	116.0
114.90	204.0
115.80	400.0
116.80	852.0
117.90	525.0
118.80	724.0
123.90	149.0
125.00	131.0
127.80	367.0
128.80	227.0
129.70	395.0
130.00	389.0
130.80	182.0
134.80	249.0
136.90	245.0
139.90	121.0
140.90	1535.0
141.80	252.0
142.90	1365.0
144.10	124.0
144.90	269.0
145.90	182.0
147.60	207.0
148.00	198.0
149.70	204.0
152.80	211.0
155.00	174.0
156.70	145.0
158.80	262.0
160.90	130.0
170.80	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

172.00	1132.0
173.00	1287.0
173.90	76776.0
174.90	6215.0
175.90	73224.0
176.90	5050.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	1394.0
37.00	5459.0
38.00	4760.0
39.00	2153.0
40.00	427.0
41.20	123.0
41.80	143.0
42.30	103.0
42.90	234.0
43.90	1052.0
45.00	935.0
46.00	266.0
47.10	836.0
47.90	913.0
49.00	4688.0
50.00	19968.0
51.00	6002.0
52.00	326.0
53.00	293.0
55.10	395.0
56.00	1861.0
57.00	3108.0
58.00	177.0
59.90	1245.0
61.00	5364.0
62.00	5582.0
63.00	4332.0
64.00	587.0
65.00	1021.0
66.10	179.0
67.00	473.0
68.00	10790.0
69.00	11197.0
70.00	798.0
71.10	100.0
72.00	553.0
73.00	4705.0
74.00	19936.0
75.00	53952.0
76.00	5010.0
76.90	609.0
78.10	459.0
78.90	3568.0
80.00	1114.0
80.90	3572.0
81.90	818.0
82.80	135.0
84.00	126.0
87.00	3988.0
87.90	3556.0
90.80	499.0
92.00	3123.0
93.00	4790.0
94.00	13013.0
95.00	102040.0
96.00	7220.0
97.00	261.0
103.90	570.0
105.00	163.0
105.90	620.0
106.80	231.0
110.90	114.0
112.20	101.0
112.80	129.0
113.40	111.0
114.80	202.0
115.80	437.0
116.80	943.0
117.90	537.0
118.90	758.0
119.80	115.0
123.90	197.0
127.80	388.0
128.80	280.0
129.80	376.0
129.90	373.0
130.80	222.0
134.70	217.0
135.00	190.0
136.80	292.0
139.60	108.0
140.00	132.0
140.90	1597.0
141.80	300.0
142.90	1508.0
143.70	118.0
144.00	119.0
144.90	251.0
145.80	185.0
147.70	220.0
147.90	230.0
148.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

149.80	195.0
152.80	224.0
154.80	201.0
156.70	165.0
158.90	223.0
160.80	183.0
170.10	135.0
170.80	165.0
171.90	1318.0
172.90	1423.0
173.90	84656.0
174.90	6487.0
175.90	81160.0
176.90	5277.0
178.10	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	1295.0
37.00	5132.0
38.00	4528.0
39.00	1850.0
40.00	440.0
40.90	153.0
41.80	112.0
42.30	114.0
43.00	221.0
43.90	1006.0
45.00	923.0
46.00	270.0
47.00	818.0
47.90	761.0
49.00	4555.0
50.00	18784.0
51.00	5869.0
52.00	313.0
52.90	248.0
55.00	356.0
56.00	1610.0
57.00	3026.0
58.00	186.0
59.90	1119.0
61.00	5199.0
62.00	5216.0
63.00	4098.0
64.00	590.0
65.00	1105.0
66.10	130.0
67.00	354.0
68.00	10364.0
69.00	10913.0
70.00	769.0
71.00	115.0
72.00	528.0
73.00	4470.0
74.00	18728.0
75.00	52400.0
76.00	4512.0
76.90	531.0
78.00	363.0
78.90	3605.0
79.90	978.0
80.90	3426.0
81.90	829.0
82.80	143.0
85.70	107.0
87.00	3844.0
87.90	3328.0
90.80	497.0
92.00	3148.0
93.00	5046.0
94.00	12309.0
95.00	98392.0
96.00	6809.0
97.00	276.0
102.90	107.0
103.80	459.0
104.80	141.0
105.10	135.0
105.90	645.0
106.70	240.0
108.40	104.0
109.90	110.0
110.80	136.0
112.90	165.0
113.50	109.0
114.90	195.0
115.80	453.0
116.90	962.0
117.80	492.0
118.90	731.0
119.80	102.0
123.90	184.0
127.90	393.0
128.80	295.0
129.90	380.0
130.80	248.0
134.70	186.0
135.80	109.0
136.80	302.0
139.60	104.0
140.00	126.0
140.90	1484.0
141.80	292.0
143.00	1483.0
143.90	112.0
144.70	248.0
145.00	249.0
145.80	224.0
147.80	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

148.80	131.0
149.90	218.0
152.80	182.0
153.70	104.0
154.70	257.0
156.70	164.0
158.90	201.0
160.90	198.0
170.10	157.0
170.70	180.0
171.90	1320.0
172.90	1438.0
173.90	84784.0
174.90	6054.0
175.90	80944.0
177.00	5148.0
178.10	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.30	135.0
37.10	117.0
37.80	133.0
39.90	395.0
40.60	104.0
41.30	120.0
41.90	137.0
42.90	133.0
43.20	123.0
43.90	365.0
44.60	125.0
48.70	108.0
54.70	145.0
55.80	121.0
58.90	136.0
65.90	126.0
66.90	148.0
67.70	105.0
84.90	130.0
89.00	106.0
89.90	104.0
105.80	103.0
107.20	116.0
222.50	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42