

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021561.D
 Acq On : 24 Jun 2021 10:39
 Operator : SY/MD
 Sample : VV0624WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 25 03:01:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 25 03:01:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	461746	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	424874	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	210499	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	131583	43.283	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.560%		
7) Chloroethane-d5	1.568	69	112711	49.840	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.680%		
11) 1,1-Dichloroethene-d2	2.108	63	181237	34.889	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.780%		
21) 2-Butanone-d5	3.902	46	259567	119.069	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	119.070%		
24) Chloroform-d	4.352	84	282444	46.672	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.340%		
26) 1,2-Dichloroethane-d4	5.034	65	177223	50.843	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.680%		
32) Benzene-d6	5.053	84	583830	49.119	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.240%		
36) 1,2-Dichloropropane-d6	6.072	67	186678	50.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.720%		
41) Toluene-d8	7.317	98	523340	46.215	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.440%		
43) trans-1,3-Dichloroprop...	7.625	79	92524	47.102	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.200%		
47) 2-Hexanone-d5	8.092	63	173167	102.742	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.740%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	253276	49.709	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.420%		
66) 1,2-Dichlorobenzene-d4	11.625	152	204756	46.794	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.580%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.625	75	3744	0.759	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021561.D
Acq On : 24 Jun 2021 10:39
Operator : SY/MD
Sample : VV0624WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 25 03:01:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 25 03:01:05 2021
Response via : Initial Calibration

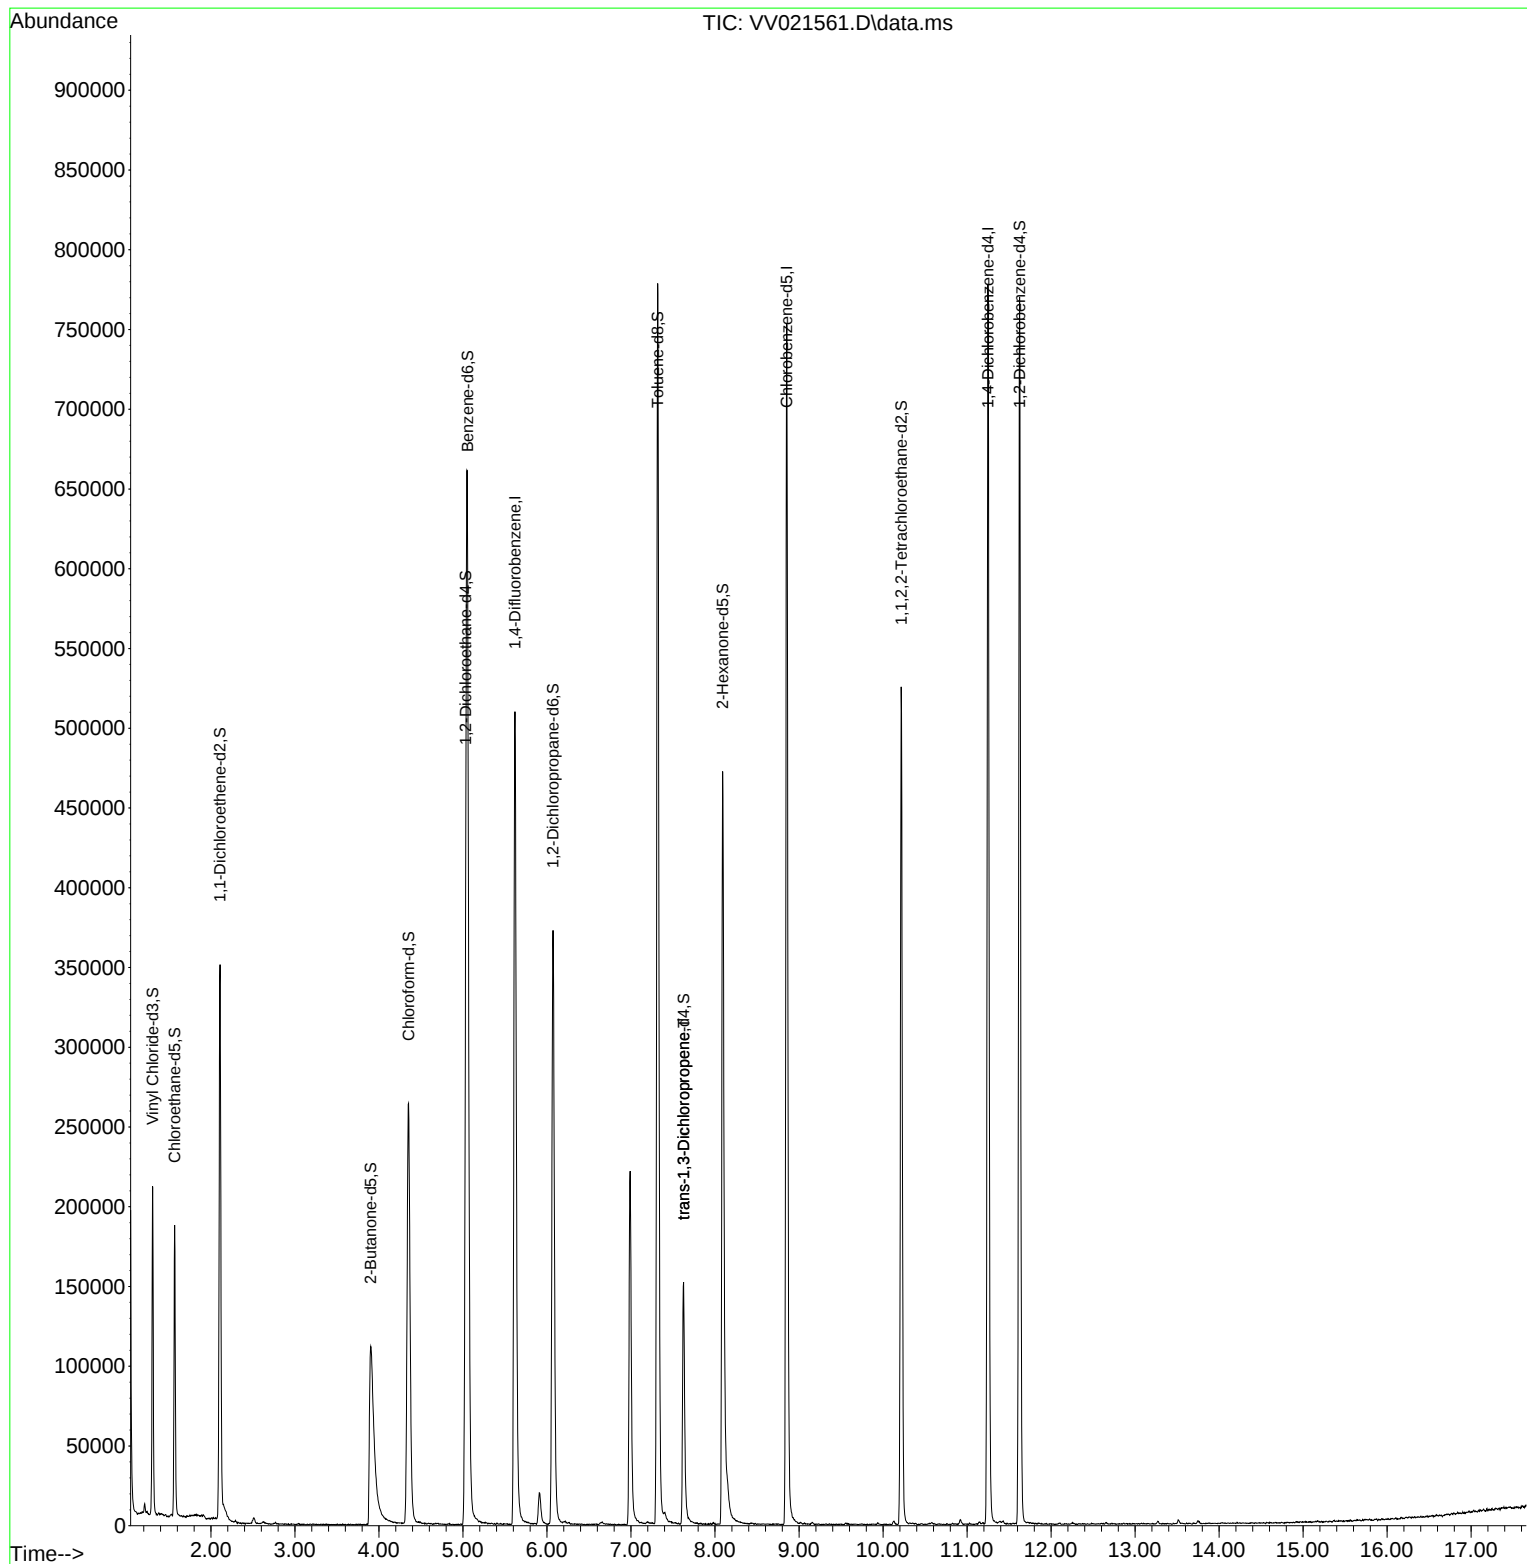

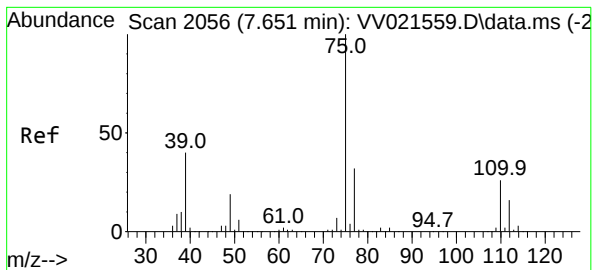

#44
 trans-1,3-Dichloropropene
 Concen: 0.759 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021561.D
 Acq: 24 Jun 2021 10:39

Instrument :
 MSVOA_V
 ClientSampleId :

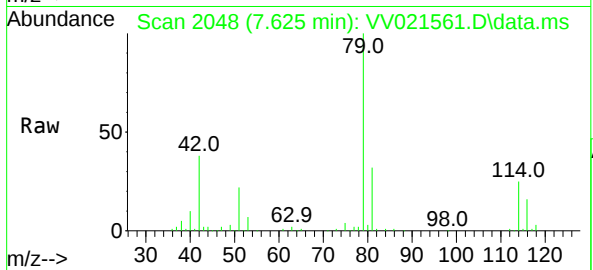

Tgt Ion: 75 Resp: 3744
 Ion Ratio Lower Upper
 75 100
 77 40.1 22.9 42.5

