

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021562.D
 Acq On : 24 Jun 2021 11:26
 Operator : SY/MD
 Sample : M2825-05ME
 Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 25 03:01:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 25 03:01:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	492342	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	471050	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	238177	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	136700	42.172	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.340%
7) Chloroethane-d5	1.568	69	107792	44.703	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.400%
11) 1,1-Dichloroethene-d2	2.089	63	134646	24.309	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.620%#
21) 2-Butanone-d5	3.905	46	159441	68.594	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	68.590%
24) Chloroform-d	4.343	84	292244	45.290	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.580%
26) 1,2-Dichloroethane-d4	5.027	65	184675	49.689	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.380%
32) Benzene-d6	5.040	84	600864	45.597	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.200%
36) 1,2-Dichloropropane-d6	6.066	67	191342	47.019	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.040%
41) Toluene-d8	7.313	98	555502	44.247	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.500%
43) trans-1,3-Dichloroprop...	7.622	79	97870	44.939	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.880%
47) 2-Hexanone-d5	8.121	63	161583	86.471	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.470%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	249824	44.225	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.440%
66) 1,2-Dichlorobenzene-d4	11.628	152	217423	43.914	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.820%
Target Compounds						Qvalue
16) Methylene chloride	2.497	84	3914	1.081	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021562.D
Acq On : 24 Jun 2021 11:26
Operator : SY/MD
Sample : M2825-05ME
Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 25 03:01:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 25 03:01:05 2021
Response via : Initial Calibration

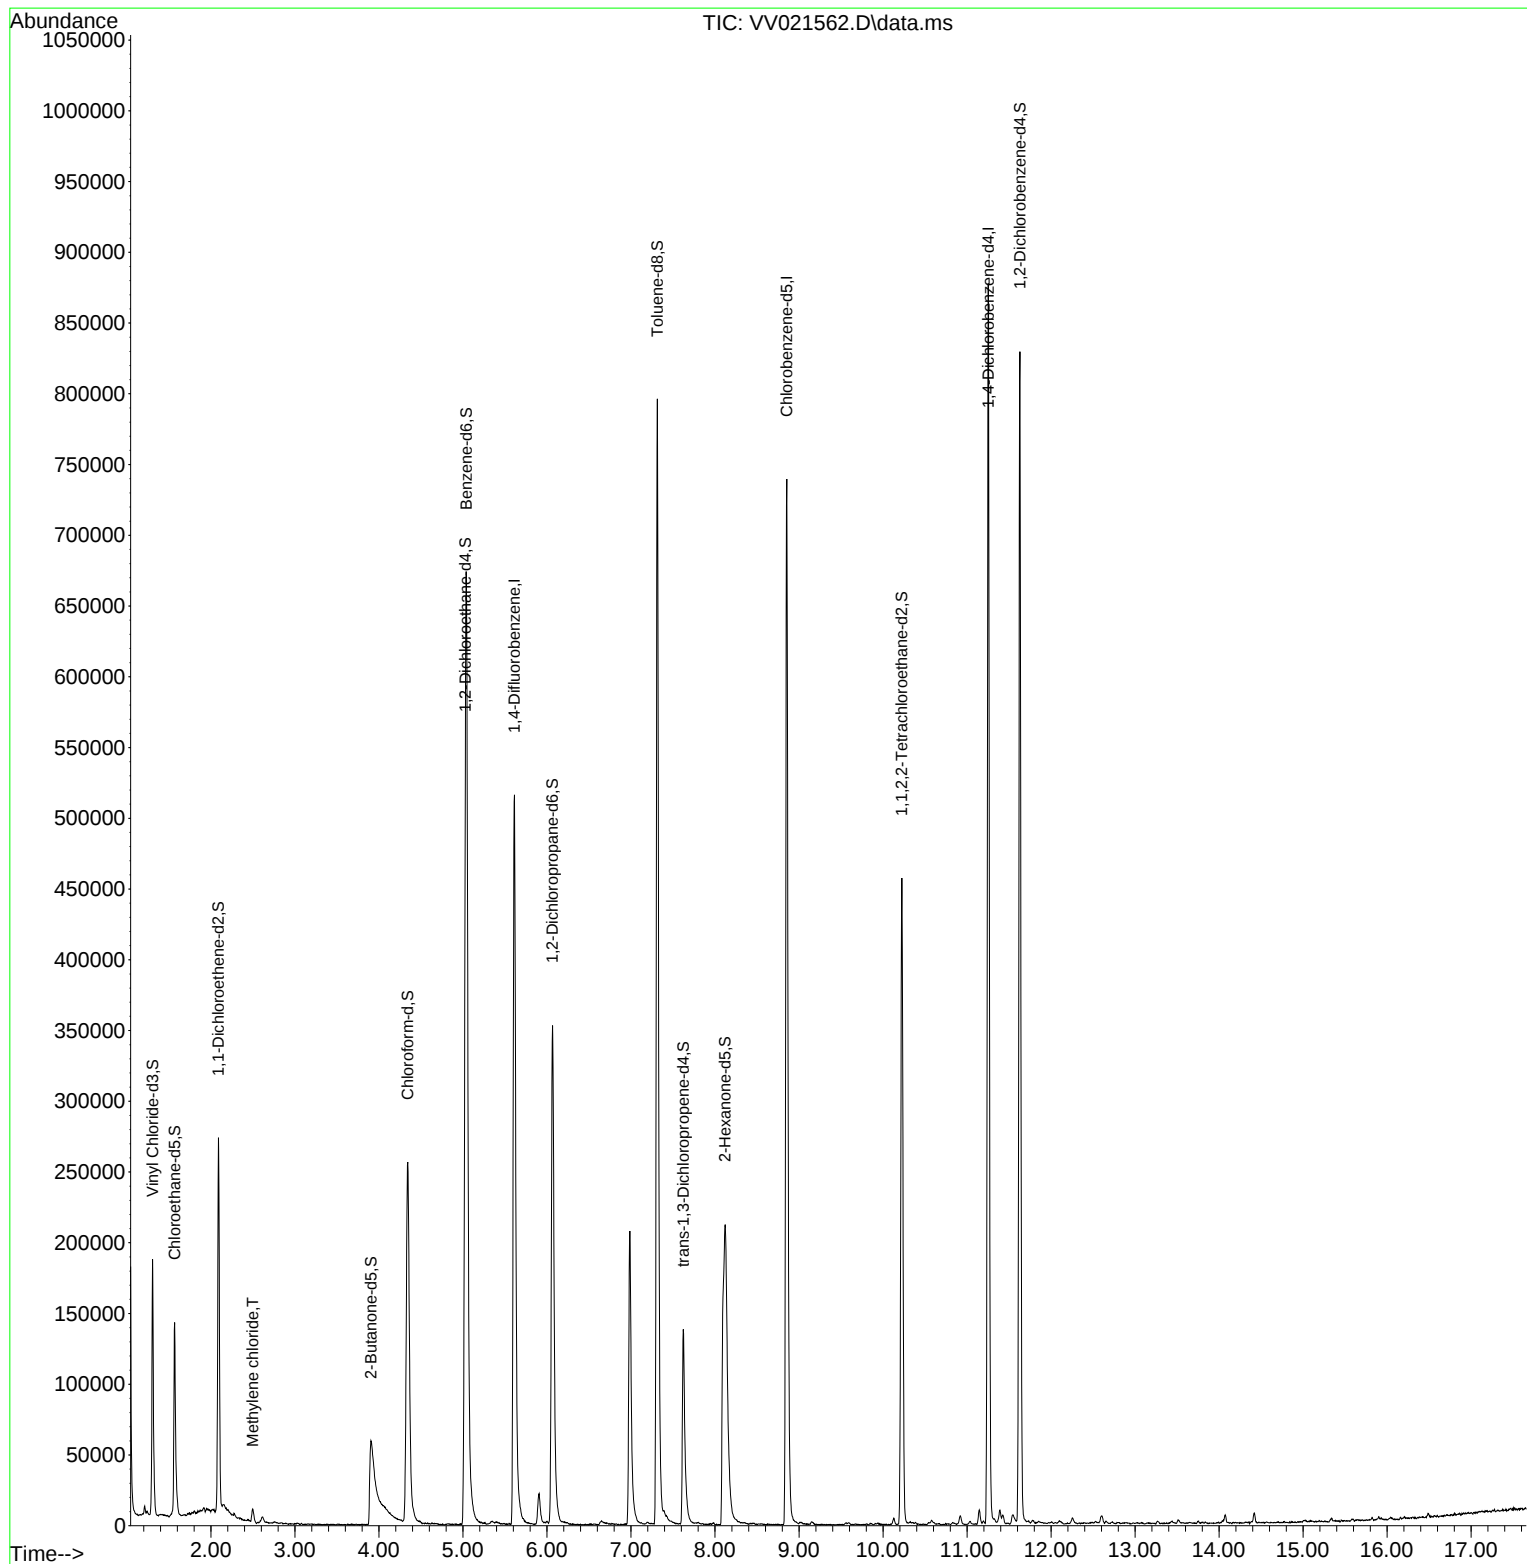

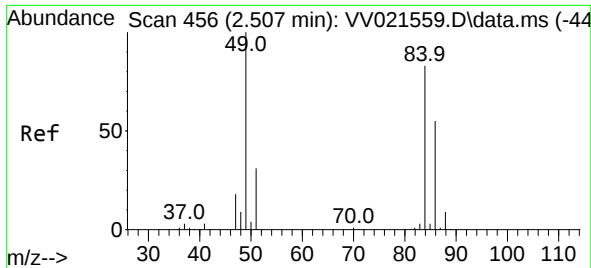

#16
Methylene chloride
Concen: 1.081 ug/L
RT: 2.497 min Scan# 453
Delta R.T. -0.010 min
Lab File: VV021562.D
Acq: 24 Jun 2021 11:26

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 84 Resp: 3914
Ion Ratio Lower Upper
84 100
86 61.7 44.1 81.9
49 114.9 80.8 150.0

