

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021560.D
 Acq On : 24 Jun 2021 10:16
 Operator : SY/MD
 Sample : VV0624MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK196

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	209770	220087	13.00%	1.668%
2	1.568	157	164	175	rVB	184356	203588	12.02%	1.543%
3	2.108	322	332	363	rVB	362579	545924	32.24%	4.136%
4	2.909	580	581	583	rBV	230	120	0.01%	0.001%
5	2.925	583	586	590	rVV2	569	507	0.03%	0.004%
6	2.992	606	607	610	rBV	425	159	0.01%	0.001%
7	3.008	610	612	614	rVB2	528	225	0.01%	0.002%
8	3.056	623	627	630	rBV3	545	590	0.03%	0.004%
9	3.137	650	652	653	rBV	259	101	0.01%	0.001%
10	3.233	679	682	685	rBV	337	262	0.02%	0.002%
11	3.272	692	694	695	rBV	322	100	0.01%	0.001%
12	3.320	707	709	710	rBV	359	154	0.01%	0.001%
13	3.359	717	721	724	rBV3	411	413	0.02%	0.003%
14	3.429	739	743	744	rBV2	268	191	0.01%	0.001%
15	3.474	755	757	760	rBV	255	158	0.01%	0.001%
16	3.529	771	774	776	rBV2	251	150	0.01%	0.001%
17	3.542	776	778	779	rBV	286	145	0.01%	0.001%
18	3.629	803	805	806	rBV	550	273	0.02%	0.002%
19	3.687	820	823	827	rBV3	397	295	0.02%	0.002%
20	3.719	832	833	834	rBV3	374	115	0.01%	0.001%
21	3.812	861	862	864	rBV	267	102	0.01%	0.001%
22	3.828	864	867	868	rBV	253	145	0.01%	0.001%
23	3.854	872	875	876	rBV2	466	270	0.02%	0.002%
24	3.899	878	889	940	rBV	102035	419065	24.75%	3.175%
25	4.349	1014	1029	1059	rBV	265975	659904	38.97%	5.000%
26	4.661	1124	1126	1127	rBV	482	174	0.01%	0.001%
27	4.761	1155	1157	1160	rBV2	524	357	0.02%	0.003%
28	4.825	1173	1177	1178	rBV2	452	264	0.02%	0.002%
29	4.876	1191	1193	1195	rVV2	489	245	0.01%	0.002%
30	4.905	1199	1202	1206	rVB	269	201	0.01%	0.002%
31	4.937	1206	1212	1213	rBV2	681	531	0.03%	0.004%
32	4.973	1221	1223	1226	rVB2	382	183	0.01%	0.001%
33	5.047	1228	1246	1273	rBV2	663420	1693187	100.00%	12.829%
34	5.478	1378	1380	1382	rBV3	542	321	0.02%	0.002%
35	5.558	1400	1405	1407	rBV2	531	321	0.02%	0.002%
36	5.616	1411	1423	1450	rBV	522963	1047730	61.88%	7.938%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021560.D
 Acq On : 24 Jun 2021 10:16
 Operator : SY/MD
 Sample : VV0624MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK196

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.908	1503	1514	1532	rBV2	19568	44202	2.61%	0.335%
38	6.069	1549	1564	1594	rBV	375238	769242	45.43%	5.828%
39	6.384	1659	1662	1663	rBV2	461	228	0.01%	0.002%
40	6.449	1678	1682	1684	rBV2	405	293	0.02%	0.002%
41	6.474	1688	1690	1693	rBV2	404	231	0.01%	0.002%
42	6.516	1696	1703	1706	rBV5	499	566	0.03%	0.004%
43	6.529	1706	1707	1709	rBV	252	106	0.01%	0.001%
44	6.555	1713	1715	1718	rVB3	391	167	0.01%	0.001%
45	6.613	1728	1733	1735	rBV	345	325	0.02%	0.002%
46	6.648	1735	1744	1745	rBV4	1565	2134	0.13%	0.016%
47	6.915	1824	1827	1829	rVB	349	189	0.01%	0.001%
48	6.931	1829	1832	1836	rBV	370	329	0.02%	0.002%
49	6.986	1838	1849	1890	rBV	225713	425296	25.12%	3.222%
50	7.317	1940	1952	1972	rBV	802162	1391590	82.19%	10.544%
51	7.622	2036	2047	2068	rBV	153376	273016	16.12%	2.069%
52	7.892	2129	2131	2134	rBV2	190	95	0.01%	0.001%
53	7.912	2134	2137	2141	rVB3	528	391	0.02%	0.003%
54	7.982	2152	2159	2161	rBV3	1326	1369	0.08%	0.010%
55	8.024	2167	2172	2175	rBV2	432	380	0.02%	0.003%
56	8.040	2175	2177	2180	rBV	525	350	0.02%	0.003%
57	8.092	2182	2193	2236	rBV	431961	861551	50.88%	6.528%
58	8.513	2321	2324	2328	rBV4	619	626	0.04%	0.005%
59	8.854	2417	2430	2451	rBV	754181	1245664	73.57%	9.438%
60	9.095	2501	2505	2509	rBV3	885	748	0.04%	0.006%
61	9.153	2517	2523	2529	rBV6	1516	1956	0.12%	0.015%
62	9.249	2552	2553	2557	rVB3	333	203	0.01%	0.002%
63	9.294	2565	2567	2569	rBV	325	127	0.01%	0.001%
64	9.320	2573	2575	2577	rBV	405	230	0.01%	0.002%
65	9.449	2613	2615	2618	rVB	345	134	0.01%	0.001%
66	9.468	2618	2621	2623	rBV2	425	279	0.02%	0.002%
67	9.484	2623	2626	2629	rVB2	250	167	0.01%	0.001%
68	9.532	2637	2641	2642	rBV2	449	315	0.02%	0.002%
69	9.545	2642	2645	2648	rBV4	851	750	0.04%	0.006%
70	9.715	2695	2698	2700	rVB3	394	220	0.01%	0.002%
71	9.776	2714	2717	2721	rVB2	292	216	0.01%	0.002%
72	9.796	2721	2723	2724	rBV	270	117	0.01%	0.001%
73	9.831	2731	2734	2738	rBV2	295	219	0.01%	0.002%
74	10.014	2789	2791	2792	rBV	295	124	0.01%	0.001%
75	10.082	2809	2812	2813	rBV	406	184	0.01%	0.001%
76	10.217	2842	2854	2875	rBV	510311	805906	47.60%	6.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021560.D
 Acq On : 24 Jun 2021 10:16
 Operator : SY/MD
 Sample : VV0624MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK196

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.452	2925	2927	2928	rBV	413	199	0.01%	0.002%
78	10.510	2942	2945	2947	rBV2	403	208	0.01%	0.002%
79	10.522	2947	2949	2950	rBV2	515	201	0.01%	0.002%
80	10.657	2988	2991	2995	rBV3	484	358	0.02%	0.003%
81	10.728	3011	3013	3015	rBV3	343	177	0.01%	0.001%
82	10.764	3022	3024	3025	rBV	273	109	0.01%	0.001%
83	10.828	3041	3044	3046	rBV2	664	358	0.02%	0.003%
84	10.921	3062	3073	3081	rBV9	3915	6709	0.40%	0.051%
85	11.002	3094	3098	3102	rBV2	426	353	0.02%	0.003%
86	11.108	3127	3131	3136	rVB2	463	358	0.02%	0.003%
87	11.188	3151	3156	3164	rBV6	2738	3778	0.22%	0.029%
88	11.249	3164	3175	3195	rBV	819016	1263992	74.65%	9.577%
89	11.477	3244	3246	3249	rVB3	674	343	0.02%	0.003%
90	11.506	3253	3255	3257	rBV	365	179	0.01%	0.001%
91	11.548	3265	3268	3272	rVB4	723	576	0.03%	0.004%
92	11.574	3273	3276	3279	rBV5	704	576	0.03%	0.004%
93	11.625	3280	3292	3312	rBV	788807	1251559	73.92%	9.483%
94	11.783	3339	3341	3345	rBV3	979	690	0.04%	0.005%
95	12.452	3548	3549	3552	rVB	309	107	0.01%	0.001%
96	12.651	3605	3611	3619	rVB4	4332	6114	0.36%	0.046%
97	12.876	3678	3681	3684	rBV3	482	317	0.02%	0.002%
98	13.272	3796	3804	3812	rBV5	6141	8943	0.53%	0.068%
99	13.513	3871	3879	3891	rVB	9056	15183	0.90%	0.115%
100	13.747	3945	3952	3962	rVB4	7003	9998	0.59%	0.076%


Sum of corrected areas: 13198177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021560.D
Acq On : 24 Jun 2021 10:16
Operator : SY/MD
Sample : VV0624MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

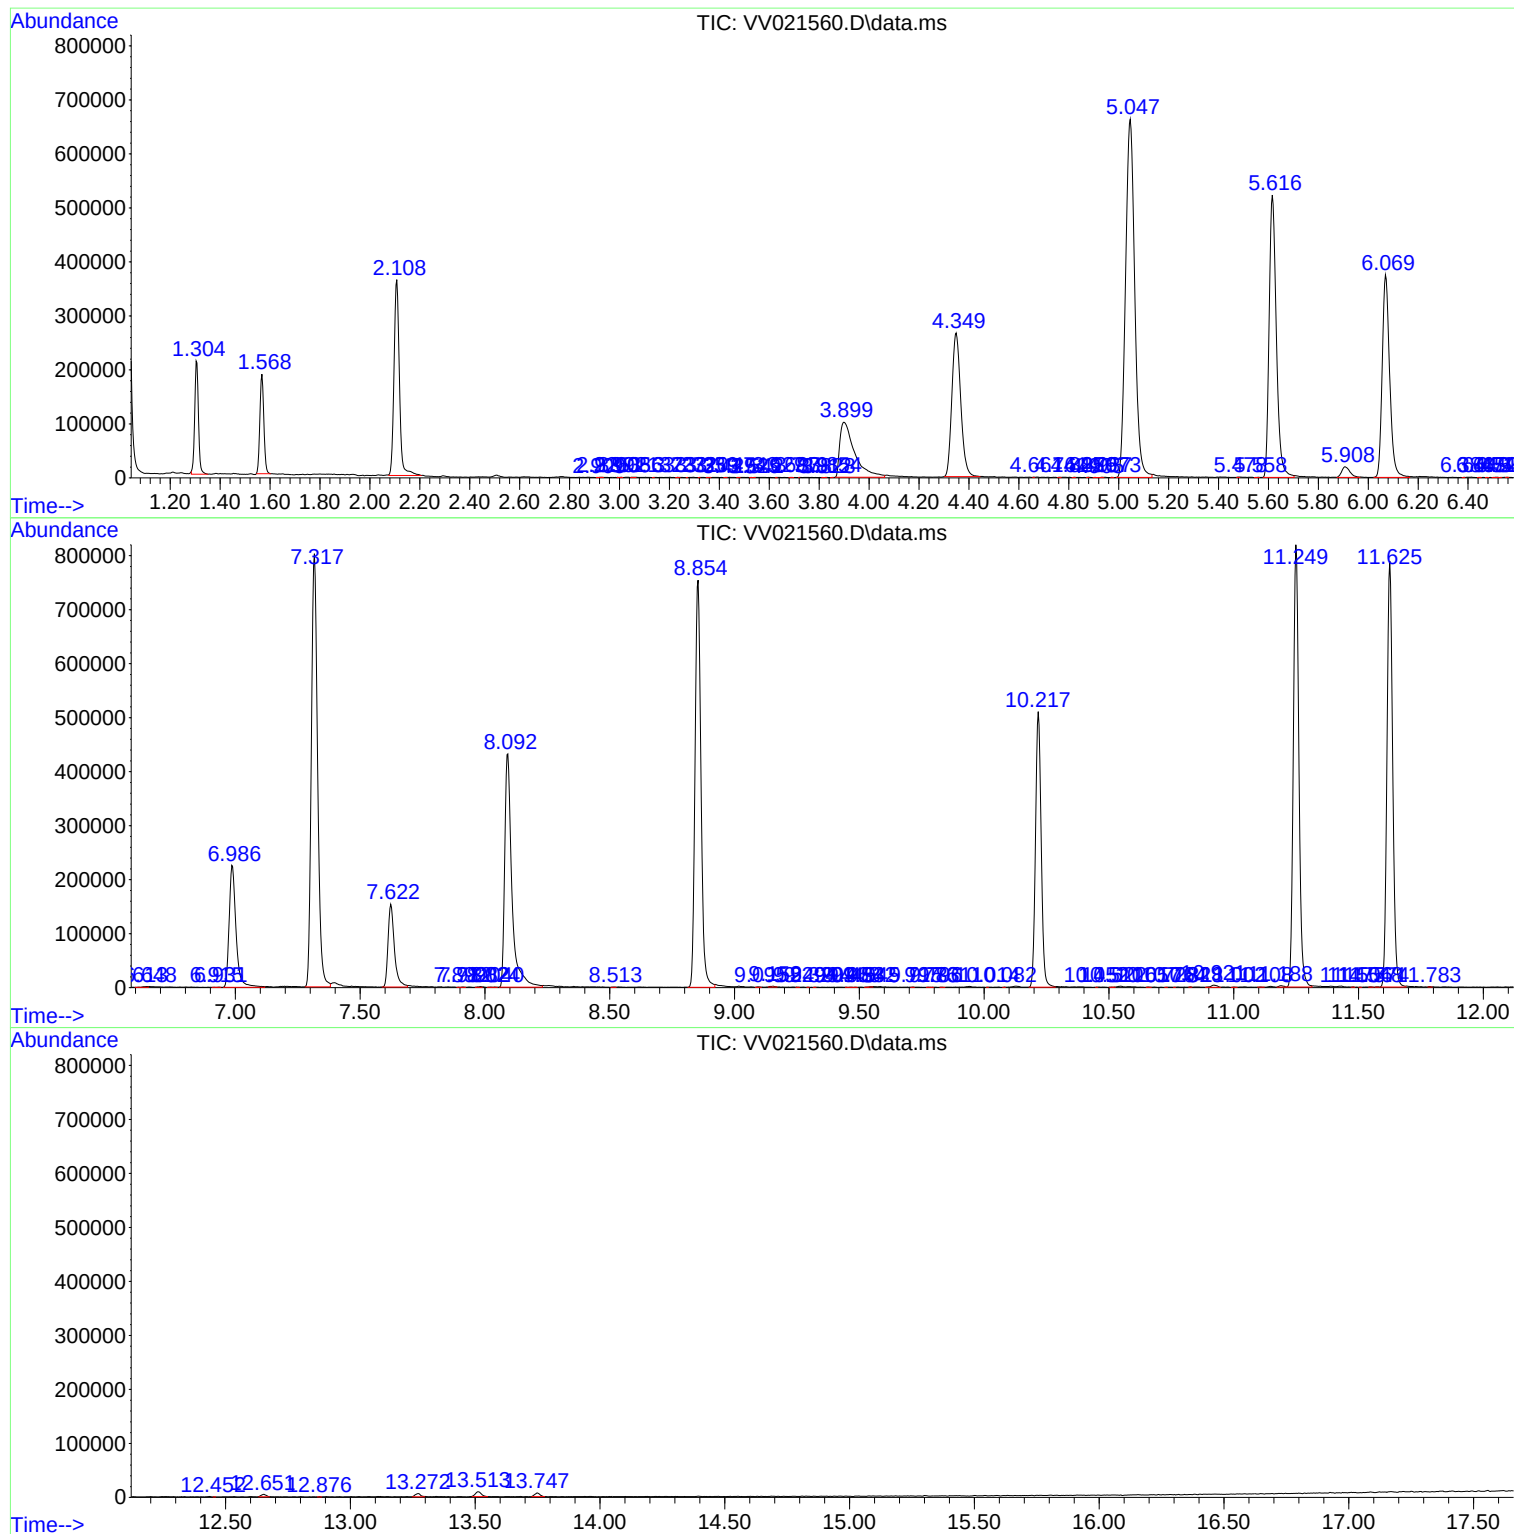

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021560.D
Acq On : 24 Jun 2021 10:16
Operator : SY/MD
Sample : VV0624MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021560.D
Acq On : 24 Jun 2021 10:16
Operator : SY/MD
Sample : VV0624MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
