

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021562.D
 Acq On : 24 Jun 2021 11:26
 Operator : SY/MD
 Sample : M2825-05ME
 Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDQ9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	180937	224130	12.87%	1.681%
2	1.568	157	164	187	rVB	136523	196397	11.27%	1.473%
3	2.089	319	326	340	rVB	260457	355834	20.43%	2.668%
4	2.999	606	609	611	rBV3	611	307	0.02%	0.002%
5	3.076	628	633	634	rBV2	958	712	0.04%	0.005%
6	3.114	643	645	647	rBV2	377	183	0.01%	0.001%
7	3.307	704	705	708	rVB	279	109	0.01%	0.001%
8	3.339	713	715	718	rVB2	233	101	0.01%	0.001%
9	3.355	718	720	723	rVB3	298	139	0.01%	0.001%
10	3.375	723	726	729	rBV3	394	255	0.01%	0.002%
11	3.391	729	731	734	rBV3	320	175	0.01%	0.001%
12	3.423	738	741	743	rBV	453	303	0.02%	0.002%
13	3.503	761	766	772	rBV5	459	585	0.03%	0.004%
14	3.671	815	818	822	rVB3	512	297	0.02%	0.002%
15	3.690	822	824	828	rVB3	619	324	0.02%	0.002%
16	3.709	828	830	831	rBV	392	185	0.01%	0.001%
17	3.751	841	843	849	rVB3	456	441	0.03%	0.003%
18	3.780	849	852	854	rBV	361	275	0.02%	0.002%
19	3.854	872	875	879	rBV3	499	431	0.02%	0.003%
20	3.905	879	891	931	rBV	59397	295376	16.96%	2.215%
21	4.343	1013	1027	1066	rVB	254074	674614	38.73%	5.059%
22	4.757	1154	1156	1160	rVB2	720	306	0.02%	0.002%
23	4.799	1163	1169	1171	rBV3	530	527	0.03%	0.004%
24	4.854	1184	1186	1187	rVB	303	101	0.01%	0.001%
25	4.867	1189	1190	1191	rVB	206	40	0.00%	0.000%
26	4.876	1191	1193	1196	rBV3	456	273	0.02%	0.002%
27	4.963	1218	1220	1221	rBV3	378	161	0.01%	0.001%
28	5.040	1227	1244	1283	rBV2	673110	1742024	100.00%	13.063%
29	5.555	1397	1404	1406	rVB3	828	858	0.05%	0.006%
30	5.568	1406	1408	1409	rBV	373	135	0.01%	0.001%
31	5.613	1409	1422	1454	rBV	515560	1104375	63.40%	8.282%
32	5.905	1501	1513	1531	rBV2	21577	47568	2.73%	0.357%
33	6.066	1550	1563	1596	rBV	350859	777006	44.60%	5.827%
34	6.281	1627	1630	1633	rVB2	514	273	0.02%	0.002%
35	6.349	1650	1651	1652	rBV	320	106	0.01%	0.001%
36	6.397	1661	1666	1668	rBV3	600	459	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021562.D
 Acq On : 24 Jun 2021 11:26
 Operator : SY/MD
 Sample : M2825-05ME
 Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDQ9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.436	1677	1678	1680	rBV	197	70	0.00%	0.001%
38	6.455	1682	1684	1686	rVV2	452	188	0.01%	0.001%
39	6.481	1690	1692	1693	rBV	193	86	0.00%	0.001%
40	6.490	1693	1695	1697	rVB	353	145	0.01%	0.001%
41	6.506	1697	1700	1702	rBV3	690	386	0.02%	0.003%
42	6.516	1702	1703	1706	rVV2	372	155	0.01%	0.001%
43	6.635	1736	1740	1741	rBV	1649	1147	0.07%	0.009%
44	6.847	1803	1806	1809	rBV2	502	209	0.01%	0.002%
45	6.883	1813	1817	1818	rBV3	586	407	0.02%	0.003%
46	6.986	1837	1849	1880	rBV	207338	430973	24.74%	3.232%
47	7.313	1939	1951	1973	rBV	795230	1443680	82.87%	10.826%
48	7.622	2036	2047	2081	rBV	137589	292522	16.79%	2.194%
49	7.931	2139	2143	2145	rBV3	771	563	0.03%	0.004%
50	7.947	2146	2148	2151	rVB	705	381	0.02%	0.003%
51	7.966	2151	2154	2155	rBV3	573	346	0.02%	0.003%
52	8.021	2169	2171	2174	rVB3	489	193	0.01%	0.001%
53	8.040	2174	2177	2180	rBV2	349	244	0.01%	0.002%
54	8.121	2184	2202	2249	rBV3	212117	834831	47.92%	6.260%
55	8.423	2290	2296	2297	rBV5	808	810	0.05%	0.006%
56	8.516	2321	2325	2326	rBV3	516	341	0.02%	0.003%
57	8.587	2344	2347	2350	rVB2	511	322	0.02%	0.002%
58	8.693	2378	2380	2381	rBV	263	81	0.00%	0.001%
59	8.748	2394	2397	2401	rBV3	419	293	0.02%	0.002%
60	8.767	2401	2403	2406	rVB2	331	115	0.01%	0.001%
61	8.796	2408	2412	2413	rBV2	361	235	0.01%	0.002%
62	8.854	2418	2430	2455	rBV	739015	1358985	78.01%	10.191%
63	9.101	2505	2507	2510	rBV3	477	305	0.02%	0.002%
64	9.153	2516	2523	2526	rBV4	2018	2598	0.15%	0.019%
65	9.207	2535	2540	2543	rBV4	441	363	0.02%	0.003%
66	9.239	2548	2550	2552	rVB2	313	122	0.01%	0.001%
67	9.265	2554	2558	2560	rBV2	508	329	0.02%	0.002%
68	9.301	2566	2569	2570	rBV	194	107	0.01%	0.001%
69	9.329	2574	2578	2579	rBV	342	134	0.01%	0.001%
70	9.387	2595	2596	2597	rVB	137	26	0.00%	0.000%
71	9.403	2598	2601	2602	rBV	421	152	0.01%	0.001%
72	9.436	2609	2611	2613	rBV	152	91	0.01%	0.001%
73	9.455	2613	2617	2618	rVV2	214	155	0.01%	0.001%
74	9.477	2622	2624	2625	rVV	356	134	0.01%	0.001%
75	9.487	2625	2627	2631	rVB2	257	167	0.01%	0.001%
76	9.529	2637	2640	2641	rBV	209	107	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021562.D
 Acq On : 24 Jun 2021 11:26
 Operator : SY/MD
 Sample : M2825-05ME
 Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDQ9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	9.561	2641	2650	2653	rBV5	1469	2010	0.12%	0.015%
78	9.657	2676	2680	2682	rBV2	414	337	0.02%	0.003%
79	9.751	2707	2709	2713	rVB2	320	224	0.01%	0.002%
80	9.799	2721	2724	2725	rBV2	473	253	0.01%	0.002%
81	9.847	2733	2739	2742	rBV5	935	896	0.05%	0.007%
82	9.905	2755	2757	2763	rBV5	478	484	0.03%	0.004%
83	9.960	2771	2774	2776	rVB	801	452	0.03%	0.003%
84	9.973	2776	2778	2779	rBV	470	218	0.01%	0.002%
85	10.005	2785	2788	2791	rBV2	365	256	0.01%	0.002%
86	10.021	2791	2793	2795	rVV2	383	175	0.01%	0.001%
87	10.066	2804	2807	2810	rVB	367	250	0.01%	0.002%
88	10.092	2812	2815	2817	rBV2	453	254	0.01%	0.002%
89	10.223	2843	2856	2875	rBV	456709	807022	46.33%	6.052%
90	10.413	2913	2915	2916	rBV	404	119	0.01%	0.001%
91	10.542	2950	2955	2957	rBV4	1366	1266	0.07%	0.009%
92	10.702	3003	3005	3006	rBV4	157	58	0.00%	0.000%
93	10.744	3015	3018	3021	rVB2	775	482	0.03%	0.004%
94	10.828	3036	3044	3049	rBV7	1485	2258	0.13%	0.017%
95	10.918	3066	3072	3086	rVB7	5987	10092	0.58%	0.076%
96	11.040	3101	3110	3118	rBV7	1999	3196	0.18%	0.024%
97	11.146	3134	3143	3153	rBV3	10224	17026	0.98%	0.128%
98	11.252	3165	3176	3196	rBV	876390	1384797	79.49%	10.384%
99	11.628	3282	3293	3317	rVB	826880	1302321	74.76%	9.766%
100	13.265	3797	3802	3812	rBV8	1746	3079	0.18%	0.023%




Sum of corrected areas: 13335408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021562.D
Acq On : 24 Jun 2021 11:26
Operator : SY/MD
Sample : M2825-05ME
Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDQ9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

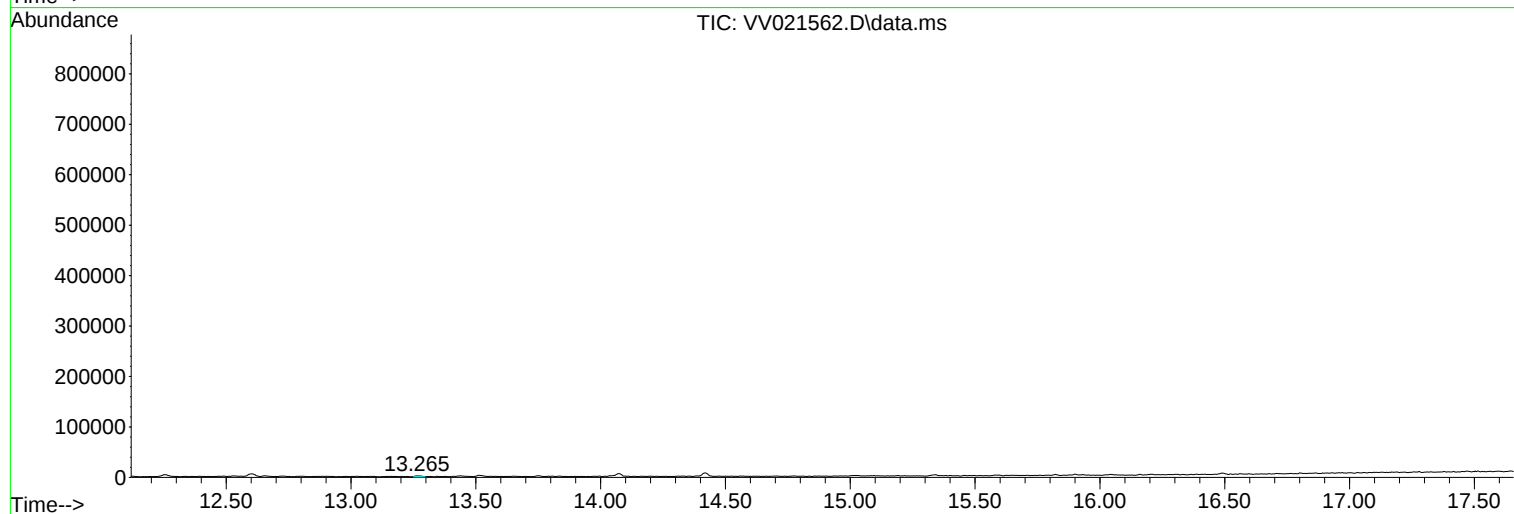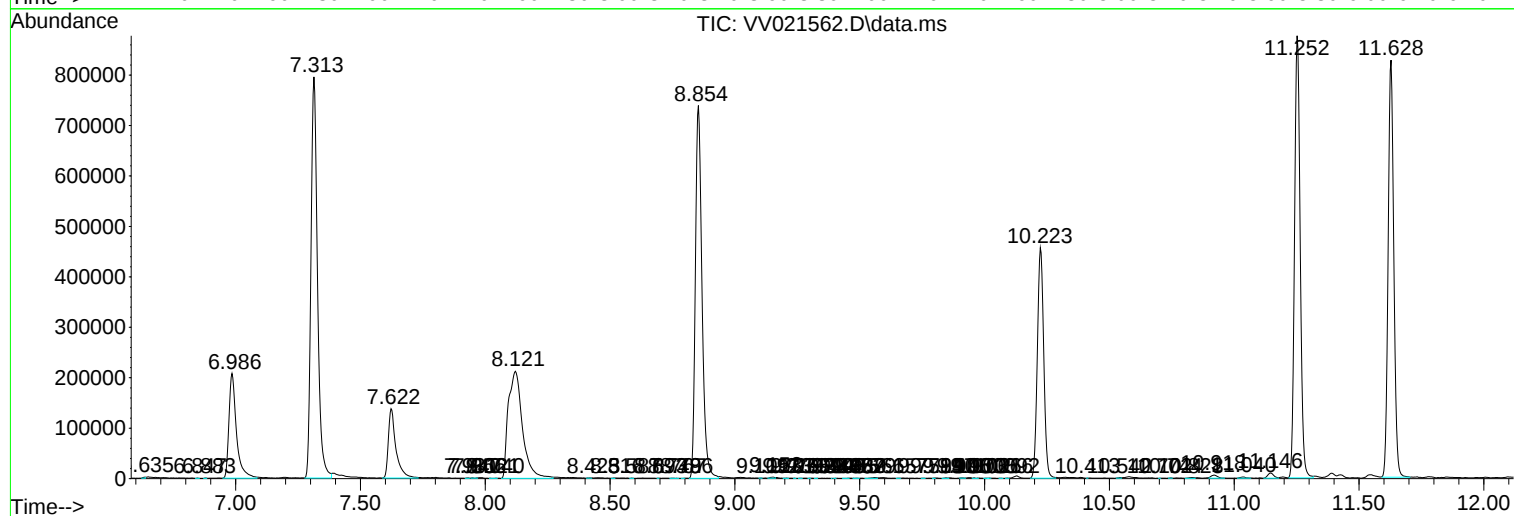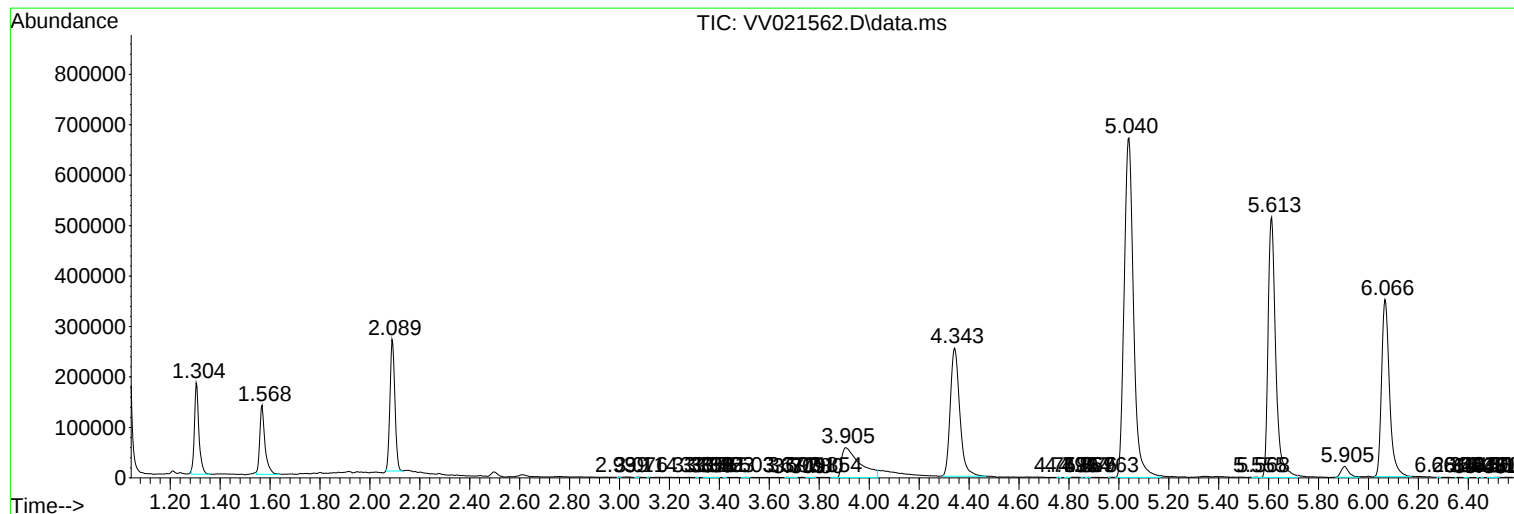

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021562.D
Acq On : 24 Jun 2021 11:26
Operator : SY/MD
Sample : M2825-05ME
Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDQ9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
Data File : VV021562.D
Acq On : 24 Jun 2021 11:26
Operator : SY/MD
Sample : M2825-05ME
Misc : 4.68g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDQ9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
