
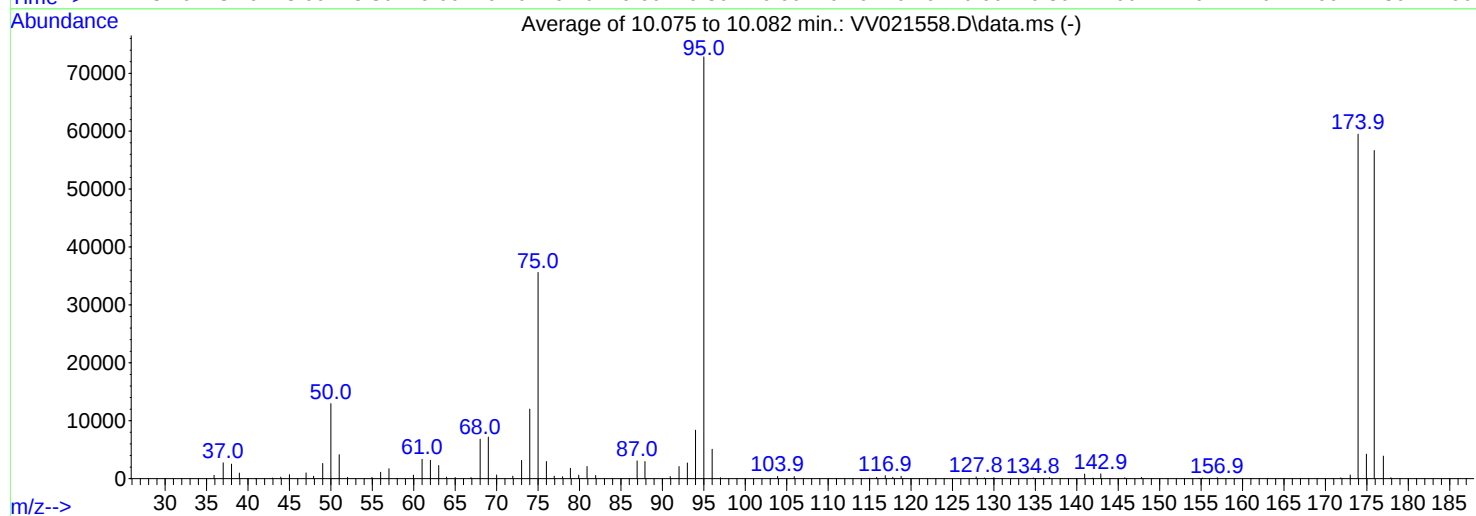


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062421\
 Data File : VV021558.D
 Acq On : 24 Jun 2021 08:43
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB172

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 25 03:01:05 2021

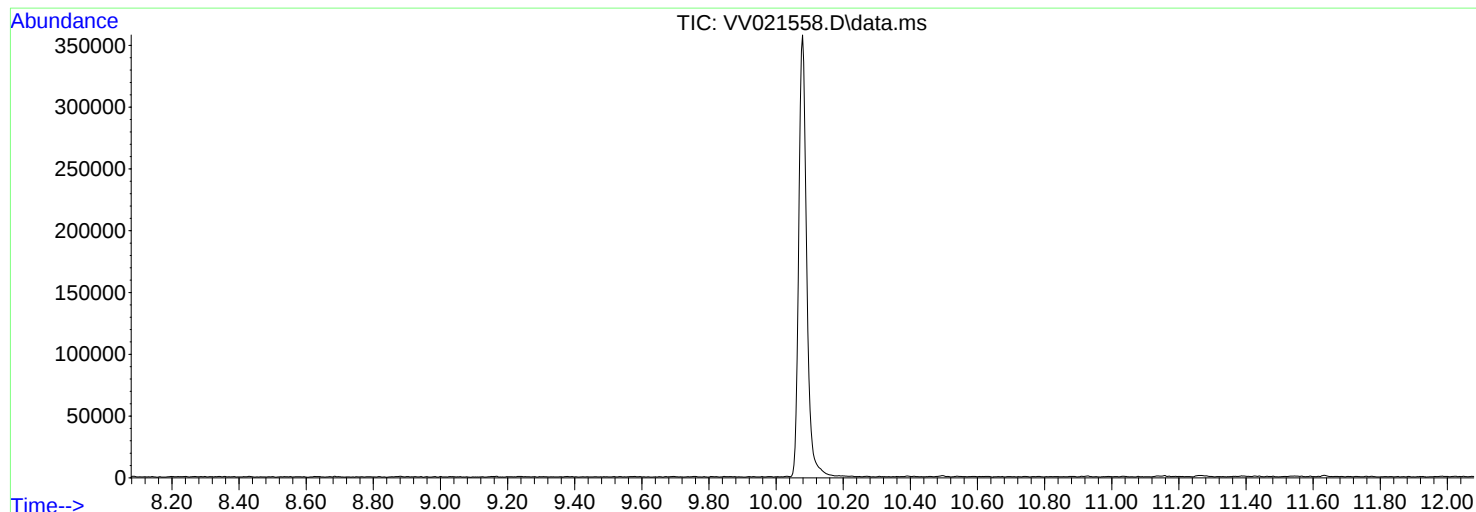

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	12965	PASS
75	95	30	80	48.9	35611	PASS
95	95	100	100	100.0	72840	PASS
96	95	5	9	7.0	5081	PASS
173	174	0.00	2	1.1	627	PASS
174	95	50	120	81.7	59491	PASS
175	174	5	9	7.1	4239	PASS
176	174	95	105	95.2	56664	PASS
177	176	5	10	6.9	3903	PASS

m/z	Abundance
35.90	595.0
37.00	2827.0
38.00	2608.0
39.00	1127.0
39.90	226.0
40.90	107.0
42.90	107.0
43.90	819.0
45.00	719.0
47.00	1083.0
47.90	471.0
49.00	2789.0
50.00	12855.0
51.00	4113.0
52.00	243.0
55.00	265.0
56.00	1085.0
57.00	1708.0
60.00	603.0
61.00	3520.0
62.00	2952.0
63.00	2407.0
64.00	246.0
65.00	202.0
66.90	194.0
68.00	6934.0
69.00	7365.0
70.00	673.0
71.90	456.0
73.00	3183.0
74.00	12328.0
75.00	36336.0
76.00	3014.0
77.00	426.0
78.00	384.0
78.90	1830.0
79.90	603.0
80.90	2130.0
81.90	514.0
87.00	2943.0
87.90	2889.0
90.90	327.0
92.00	2230.0
93.00	2778.0
94.00	8351.0
95.00	73272.0
96.00	5233.0
97.00	208.0
103.90	383.0
105.90	426.0
115.90	236.0
116.90	514.0
117.80	244.0
118.80	475.0
127.90	338.0
128.90	145.0
129.80	199.0
134.70	131.0
136.70	205.0
141.00	832.0
142.00	107.0
142.90	792.0
145.80	177.0
147.80	223.0
154.70	119.0
157.00	153.0
173.00	594.0
173.90	57904.0
174.90	3953.0
175.90	55264.0
177.00	3769.0
178.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB172

m/z	Abundance
35.90	586.0
37.00	2787.0
38.00	2579.0
39.00	1146.0
39.90	236.0
40.90	107.0
42.90	103.0
44.00	839.0
45.00	735.0
47.00	1070.0
47.90	429.0
49.00	2662.0
50.00	13462.0
51.00	4316.0
52.00	221.0
55.00	231.0
56.00	1168.0
57.00	1793.0
58.00	107.0
59.90	642.0
61.00	3455.0
62.00	3345.0
63.00	2339.0
63.90	254.0
65.00	199.0
66.90	194.0
68.00	6982.0
69.00	7495.0
70.00	657.0
71.90	453.0
73.00	3219.0
74.00	12410.0
75.00	36856.0
76.00	3022.0
76.90	462.0
78.00	320.0
78.90	1855.0
79.90	630.0
80.90	2169.0
81.90	595.0
86.90	3194.0
87.90	3050.0
90.90	373.0
92.00	2165.0
93.00	2782.0
94.00	8673.0
95.00	75384.0
96.00	5244.0
97.00	166.0
103.90	422.0
105.90	392.0
115.00	117.0
115.90	224.0
116.90	531.0
117.80	249.0
118.80	432.0
127.90	316.0
128.80	155.0
130.00	264.0
134.80	144.0
136.70	172.0
141.00	864.0
142.00	110.0
142.90	863.0
145.80	165.0
147.80	250.0
154.80	134.0
155.20	139.0
157.00	188.0
170.80	105.0
171.90	178.0
173.00	638.0
174.00	61184.0
175.00	4335.0
175.90	58440.0
177.00	4057.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB172

m/z	Abundance
35.00	537.0
37.00	2596.0
38.00	2387.0
39.00	1035.0
39.00	241.0
40.00	104.0
43.00	109.0
44.00	827.0
45.00	659.0
47.00	869.0
47.00	394.0
49.00	2398.0
50.00	12579.0
51.00	3997.0
52.00	173.0
54.00	189.0
56.00	1072.0
57.00	1673.0
57.00	104.0
59.00	547.0
61.00	3077.0
62.00	3234.0
63.00	2071.0
63.00	298.0
65.00	161.0
66.00	188.0
68.00	6525.0
69.00	6738.0
70.00	545.0
72.00	423.0
73.00	3027.0
74.00	11356.0
75.00	33640.0
76.00	2818.0
76.00	458.0
77.00	262.0
78.00	1721.0
79.00	583.0
80.00	1982.0
82.00	562.0
86.00	3060.0
87.00	2926.0
91.00	351.0
92.00	1915.0
93.00	2540.0
94.00	8066.0
95.00	69864.0
96.00	4765.0
97.00	135.0
103.00	374.0
105.00	302.0
115.00	134.0
115.00	212.0
116.00	526.0
117.00	252.0
118.00	331.0
127.00	294.0
128.00	134.0
130.00	296.0
130.00	122.0
134.00	143.0
136.00	121.0
140.00	749.0
141.00	116.0
142.00	844.0
145.00	149.0
147.00	219.0
155.00	164.0
156.00	193.0
161.00	106.0
171.00	241.0
173.00	650.0
174.00	59384.0
175.00	4430.0
175.00	56288.0
177.00	3882.0
177.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB172

m/z	Abundance
38.80	122.0
40.00	225.0
40.90	105.0
44.00	551.0

Instrument :
MSVOA_V
ClientSampleId :
BFB172