

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
 Data File : VV036249.D
 Acq On : 24 Jun 2024 16:24
 Operator : SY/MD
 Sample : P2987-03
 Misc : 5.16g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 25 04:59:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 25 04:55:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	517462	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	539094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	234901	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	144191	15.156	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.640%
7) Chloroethane-d5	1.526	69	126128	16.627	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.520%
11) 1,1-Dichloroethene-d2	2.050	65	70325	16.605	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.400%
21) 2-Butanone-d5	3.838	46	10766	4.932	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	9.860%#
24) Chloroform-d	4.243	84	269364	16.373	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.480%
26) 1,2-Dichloroethane-d4	4.937	65	148091	17.169	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	68.680%#
32) Benzene-d6	4.953	84	513151	16.013	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	64.040%
36) 1,2-Dichloropropane-d6	5.986	67	166205	16.470	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	65.880%#
41) Toluene-d8	7.240	98	432669	15.303	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	61.200%
43) trans-1,3-Dichloroprop...	7.551	79	61681	14.907	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.640%
47) 2-Hexanone-d5	8.031	63	37542	27.458	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.920%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	129543	17.179	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	68.720%
66) 1,2-Dichlorobenzene-d4	11.558	152	165895	19.259	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.040%
Target Compounds						Qvalue
35) Methylcyclohexane	5.982	83	41194	2.757	ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
Data File : VV036249.D
Acq On : 24 Jun 2024 16:24
Operator : SY/MD
Sample : P2987-03
Misc : 5.16g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 25 04:59:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 25 04:55:15 2024
Response via : Initial Calibration

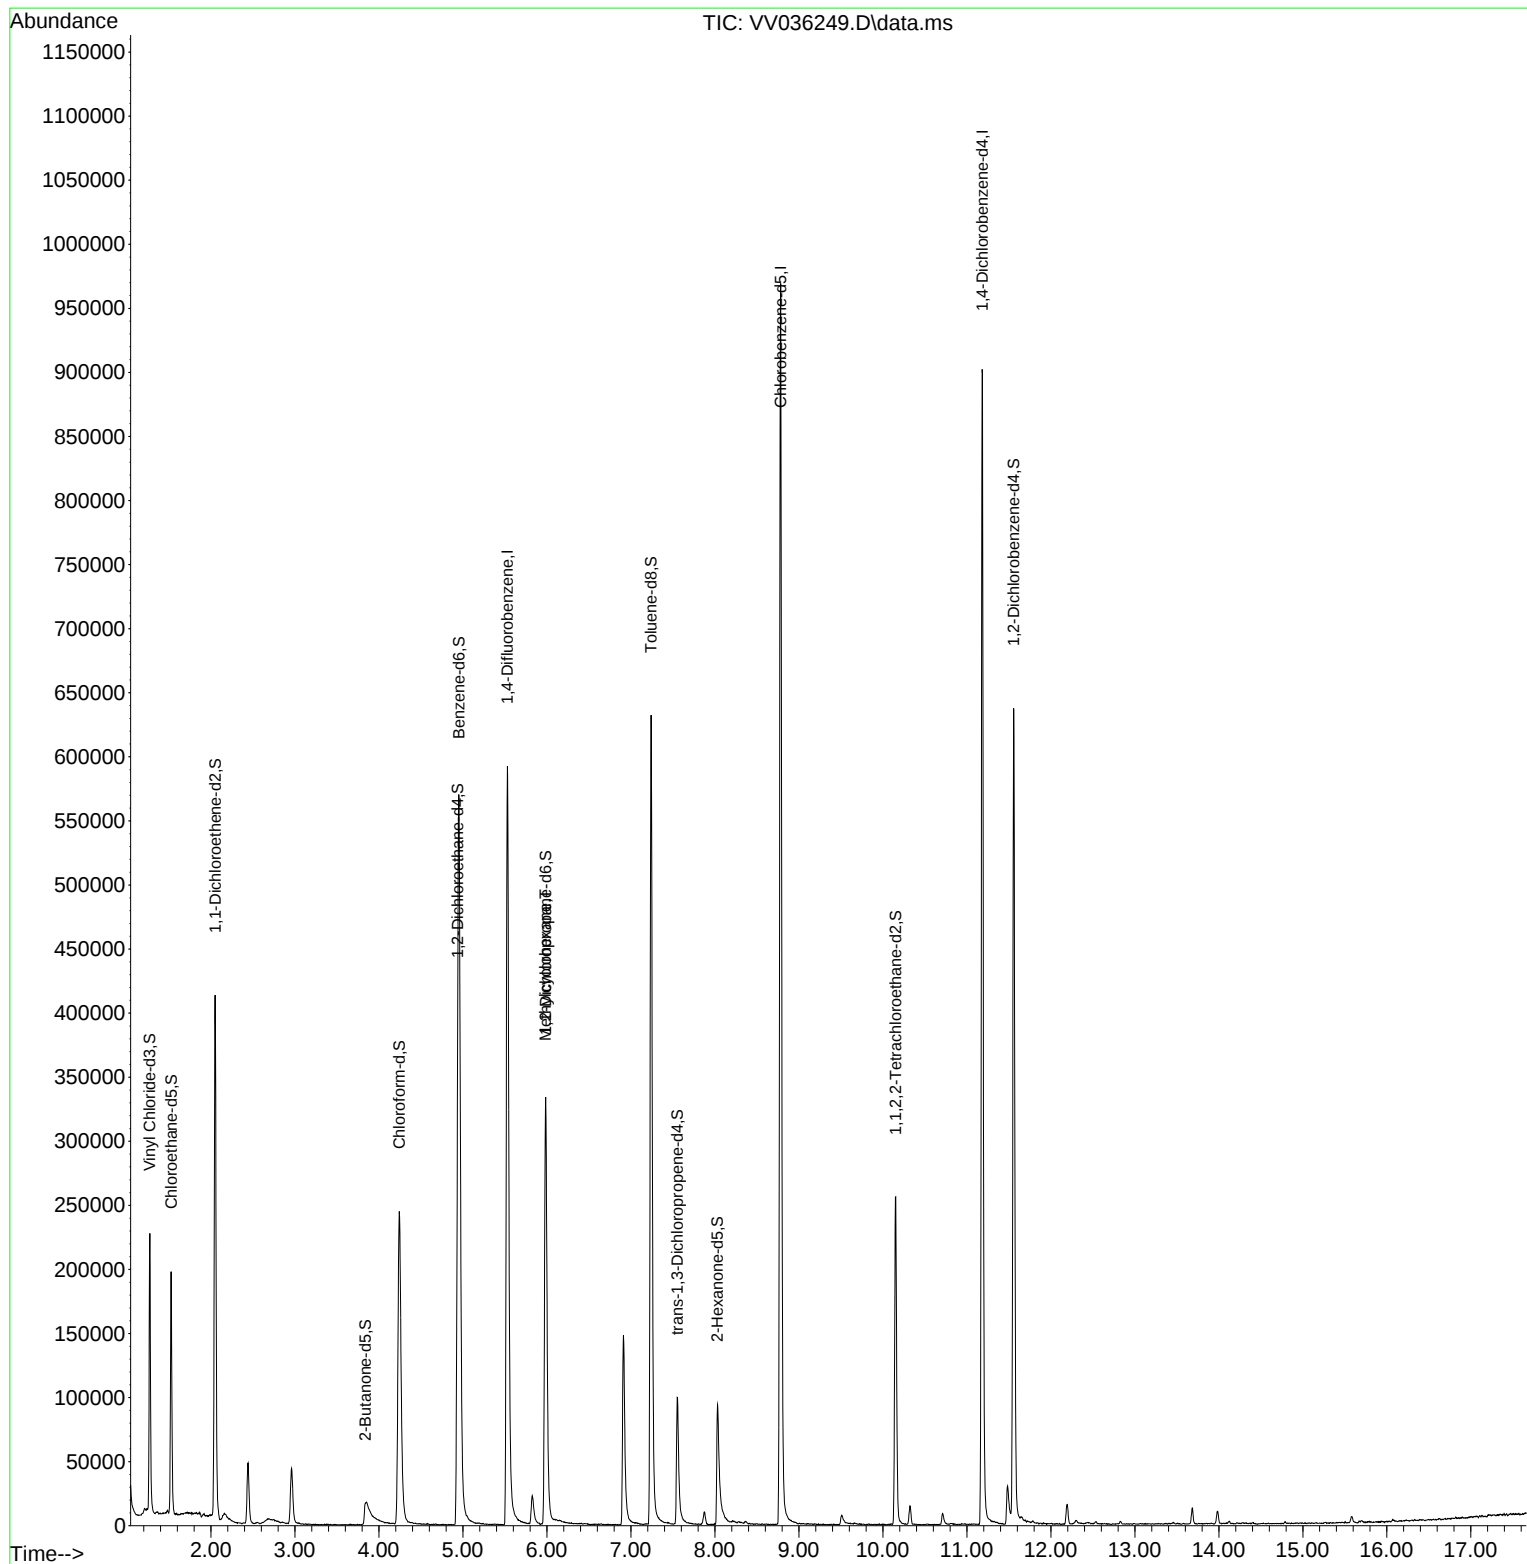

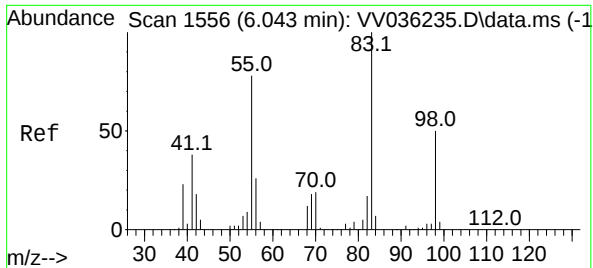

#35
Methylcyclohexane
Concen: 2.757 ug/L
RT: 5.982 min Scan# 1
Delta R.T. -0.061 min
Lab File: VV036249.D
Acq: 24 Jun 2024 16:24

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 83 Resp: 41194
Ion Ratio Lower Upper
83 100
55 0.5 60.7 91.1#
98 1.0 38.7 58.1#

