




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
Data File : VV036237.D
Acq On : 24 Jun 2024 11:40
Operator : SY/MD
Sample : P2856-13
Misc : 5.01g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SH5

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 25 04:55:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

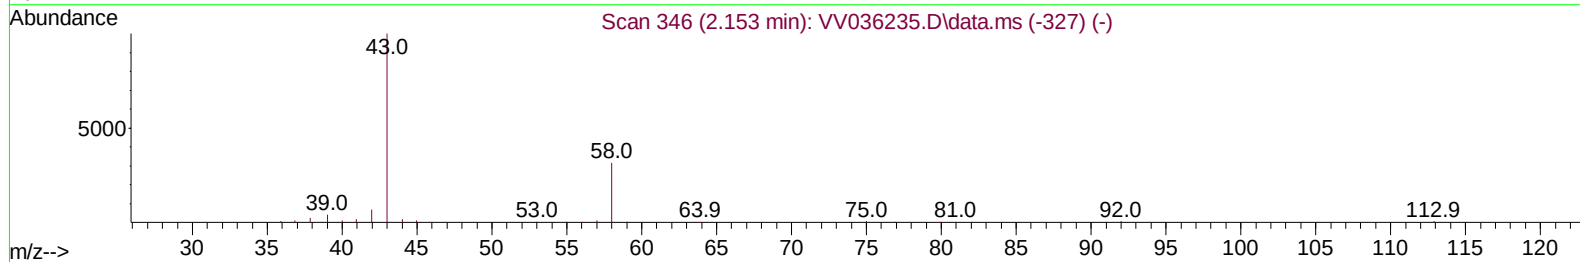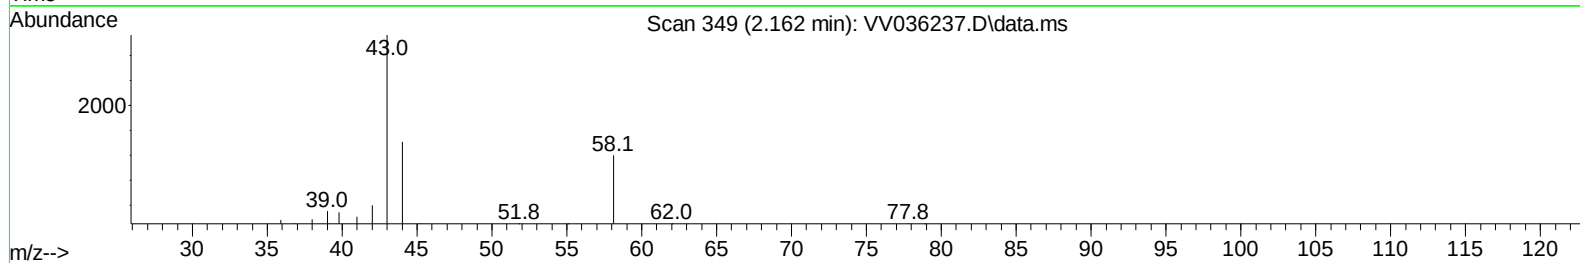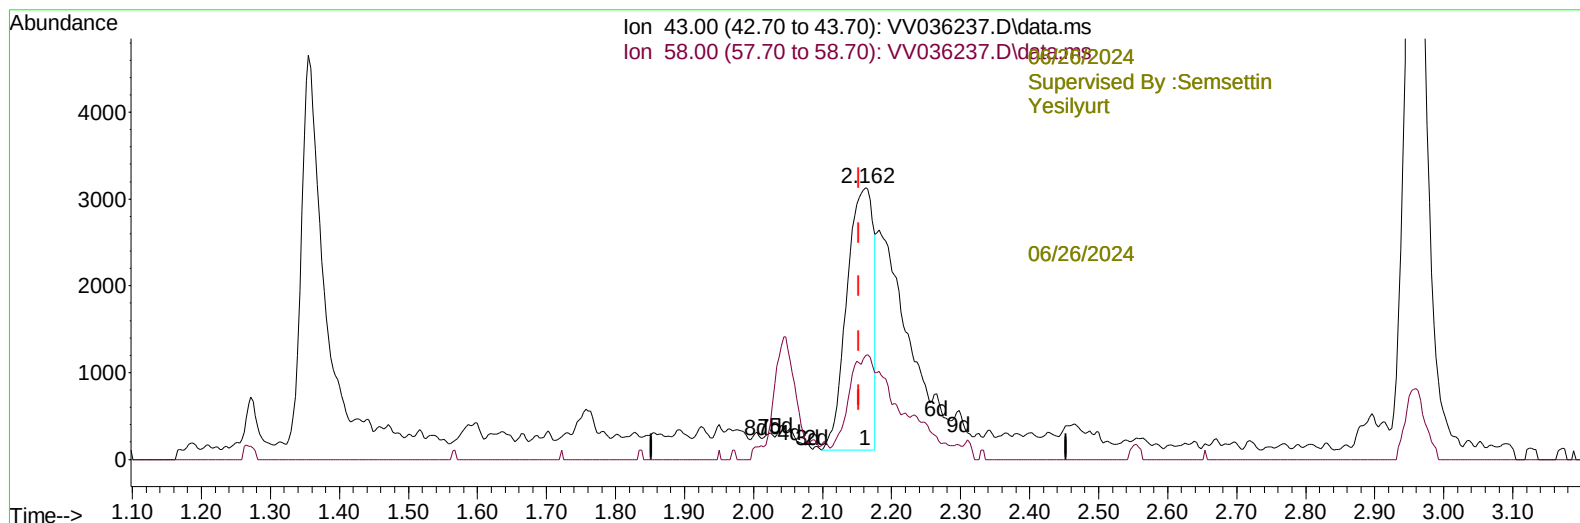

TIC: VV036237.D\data.ms

(13) Acetone (T)

2.162min (+ 0.010) 6.88 ug/L

response 8002

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	17.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
Data File : VV036237.D
Acq On : 24 Jun 2024 11:40
Operator : SY/MD
Sample : P2856-13
Misc : 5.01g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SH5

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 25 04:55:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

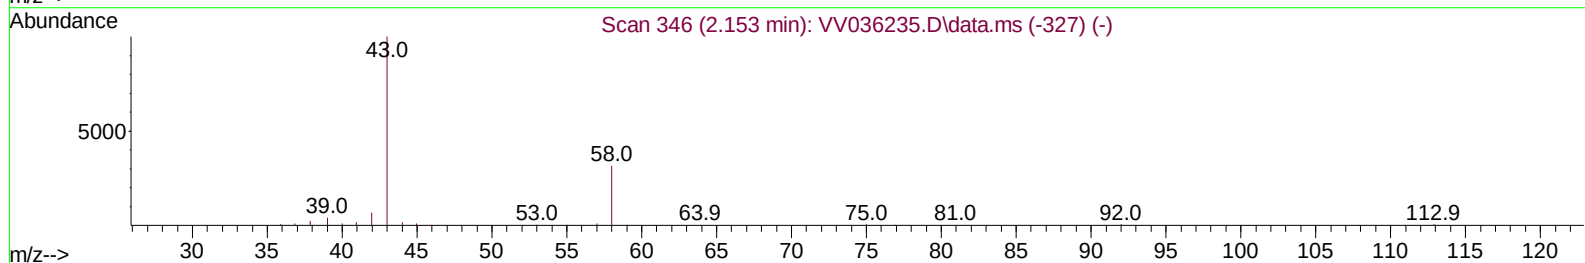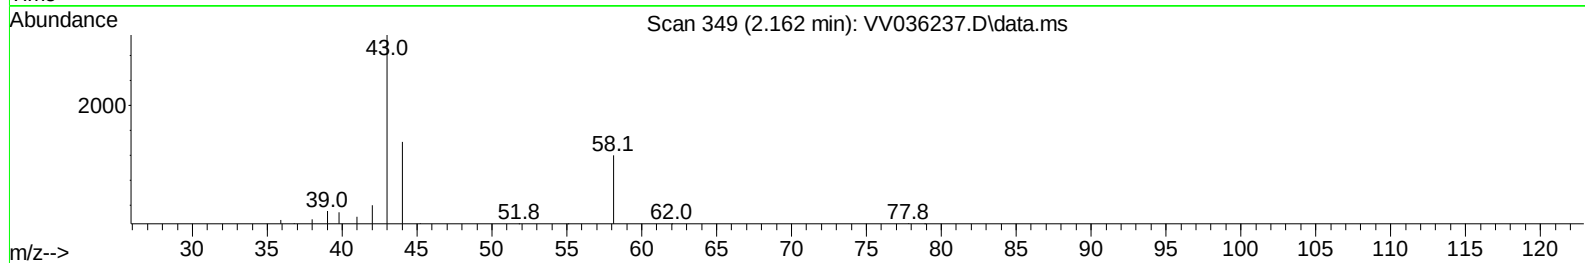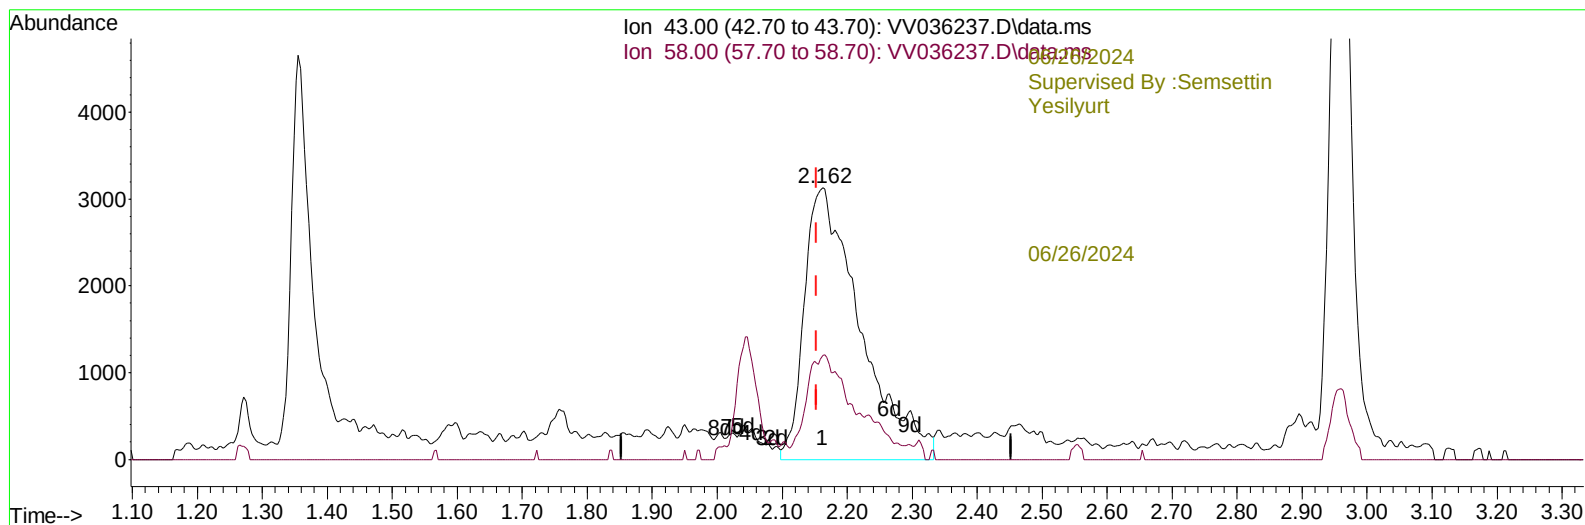

TIC: VV036237.D\data.ms

(13) Acetone (T)

2.162min (+ 0.010) 16.10 ug/L m

response 18740

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	7.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
 Data File : VV036237.D
 Acq On : 24 Jun 2024 11:40
 Operator : SY/MD
 Sample : P2856-13
 Misc : 5.01g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SH5

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:56:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 25 04:55:15 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----06/26/2024							
Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		177100	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		111834	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		21317	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		57445	17.643	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.560%	
7) Chloroethane-d5	1.526	69		58000	22.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.360%	
11) 1,1-Dichloroethene-d2	2.047	65		24300	16.765	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.040%	
21) 2-Butanone-d5	3.850	46		32060	42.916	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.840%	
24) Chloroform-d	4.243	84		117738	20.911	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.640%	
26) 1,2-Dichloroethane-d4	4.937	65		81241	27.520	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	110.080%	
32) Benzene-d6	4.953	84		191787	28.850	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.400%	
36) 1,2-Dichloropropane-d6	5.985	67		69640	33.266	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	133.080%#	
41) Toluene-d8	7.243	98		103152	17.586	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.360%	
43) trans-1,3-Dichloroprop...	7.558	79		22619	26.352	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	105.400%	
47) 2-Hexanone-d5	8.037	63		16760	59.091	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.180%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84		45698	29.212	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	116.840%	
66) 1,2-Dichlorobenzene-d4	11.564	152		11456	14.655	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	58.600%#	
Target Compounds							
13) Acetone	2.162	43		18740m	16.104	ug/L	
16) Methylene chloride	2.439	84		22110	5.517	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
Data File : VV036237.D
Acq On : 24 Jun 2024 11:40
Operator : SY/MD
Sample : P2856-13
Misc : 5.01g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SH5

Manual IntegrationsAPPROVED

Quant Time: Jun 25 04:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 25 04:55:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

