


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062424\
Data File : VV036234.D
Acq On : 24 Jun 2024 09:13
Operator : SY/MD
Sample : BFB328
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB328

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Title : VOC Analysis
Last Update : Tue Jun 25 05:53:47 2024

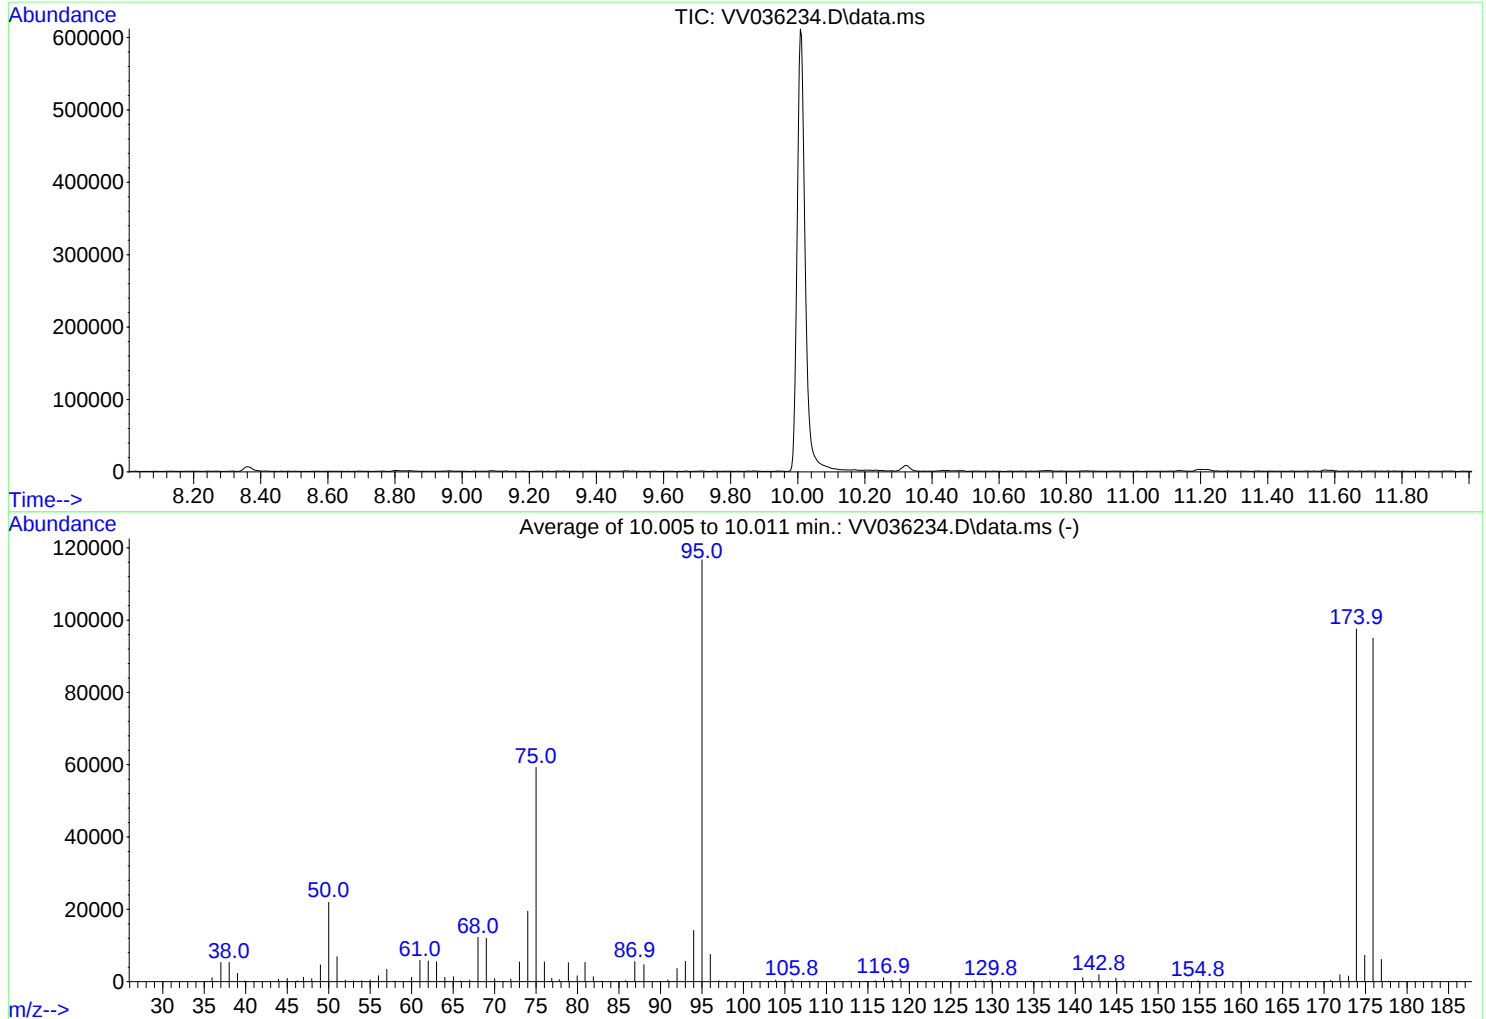

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	21936	PASS
75	95	30	80	50.8	59256	PASS
95	95	100	100	100.0	116677	PASS
96	95	5	9	6.5	7530	PASS
173	174	0.00	2	1.6	1556	PASS
174	95	50	120	83.6	97544	PASS
175	174	5	9	7.5	7313	PASS
176	174	95	101	97.4	95021	PASS
177	176	5	9	6.5	6175	PASS

m/z	Abundance
40.00	211.0
43.90	571.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
35.90	997.0
37.00	5135.0
38.00	5072.0
39.00	2126.0
39.90	456.0
43.00	127.0
44.00	1249.0
45.00	850.0
46.10	209.0
46.90	1171.0
47.90	765.0
49.00	4480.0
50.00	21352.0
51.00	6630.0
52.00	436.0
53.00	270.0
54.00	267.0
55.00	428.0
56.00	1578.0
57.00	3411.0
58.00	196.0
60.00	1118.0
61.00	5838.0
62.00	5475.0
63.00	5346.0
64.00	1182.0
65.10	1337.0
65.90	161.0
66.20	127.0
67.00	429.0
68.00	11940.0
69.00	11694.0
70.00	847.0
71.00	104.0
71.90	650.0
73.00	5426.0
74.00	18744.0
75.00	56584.0
76.00	5410.0
76.90	899.0
77.80	573.0
78.90	5017.0
79.90	1511.0
80.90	5089.0
81.90	1247.0
82.80	134.0
85.80	249.0
86.90	5351.0
88.00	4523.0
90.90	463.0
92.00	3526.0
93.00	5184.0
94.00	13511.0
95.00	111288.0
96.00	7476.0
97.10	287.0
103.90	453.0
104.80	169.0
105.80	496.0
107.90	124.0
110.90	113.0
112.70	150.0
114.60	126.0
115.70	325.0
116.90	1006.0
117.90	414.0
118.90	892.0
127.90	329.0
129.00	200.0
129.90	449.0
130.80	148.0
134.80	161.0
136.90	185.0
140.90	1050.0
141.80	145.0
142.80	1842.0
143.90	191.0
144.90	966.0
145.80	258.0
147.70	248.0
149.90	100.0
154.80	308.0
156.80	226.0
158.70	112.0
160.90	175.0
170.80	340.0
171.90	1615.0
172.90	1405.0
173.90	91344.0
174.90	6798.0
175.90	87816.0
176.90	5648.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

177.80

167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
36.00	1122.0
37.00	5371.0
38.00	5517.0
39.00	2339.0
39.90	415.0
43.00	128.0
44.00	1303.0
45.00	886.0
46.20	217.0
46.90	1207.0
47.90	851.0
49.00	4773.0
50.00	22648.0
51.00	7111.0
52.00	484.0
53.00	283.0
54.00	277.0
55.00	444.0
56.00	1666.0
57.00	3510.0
58.00	159.0
60.00	1233.0
61.00	6051.0
62.00	5931.0
63.00	5685.0
64.00	1260.0
65.00	1418.0
65.90	176.0
67.00	493.0
68.00	12744.0
69.00	12429.0
70.00	862.0
71.90	703.0
73.00	5596.0
74.00	20096.0
75.00	61184.0
76.00	5642.0
76.90	985.0
77.80	586.0
78.90	5385.0
80.00	1624.0
80.90	5502.0
81.90	1449.0
82.80	156.0
85.80	304.0
86.90	5759.0
88.00	4834.0
90.90	496.0
92.00	3771.0
93.00	5875.0
94.00	14683.0
95.00	120760.0
96.00	7736.0
97.00	276.0
103.90	482.0
105.00	168.0
105.80	487.0
107.90	143.0
110.70	103.0
110.90	102.0
112.70	167.0
114.70	115.0
115.90	399.0
116.90	1095.0
117.90	464.0
118.90	880.0
127.90	386.0
129.00	212.0
129.90	488.0
130.90	140.0
134.80	183.0
136.90	231.0
139.90	107.0
140.90	1125.0
141.80	201.0
142.90	1992.0
144.00	207.0
144.90	1001.0
145.90	206.0
146.60	105.0
147.80	290.0
149.80	132.0
153.00	112.0
154.80	306.0
156.80	208.0
158.80	127.0
160.90	159.0
170.80	414.0
171.90	1970.0
172.90	1580.0
173.90	100536.0
174.90	7571.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

175.90	98280.0
176.90	6340.0
177.80	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
36.00	1178.0
37.00	5246.0
38.00	5295.0
39.00	2328.0
39.90	392.0
42.80	104.0
44.00	1216.0
45.00	910.0
46.30	218.0
47.00	1235.0
48.00	771.0
49.00	4634.0
50.00	21808.0
51.00	6943.0
52.00	451.0
53.00	244.0
54.00	253.0
55.00	427.0
56.00	1657.0
57.00	3275.0
58.00	126.0
60.00	1192.0
61.00	5747.0
62.00	5790.0
63.00	5375.0
64.00	1191.0
65.00	1388.0
65.90	165.0
67.00	465.0
68.00	12053.0
69.00	11894.0
70.00	860.0
72.00	720.0
73.00	5268.0
74.00	19560.0
75.00	60000.0
76.00	5301.0
76.90	972.0
77.80	528.0
78.90	5288.0
80.00	1615.0
80.90	5401.0
81.90	1472.0
82.90	125.0
85.80	305.0
86.90	5469.0
88.00	4725.0
90.90	487.0
92.00	3545.0
93.00	5871.0
94.00	14313.0
95.00	117984.0
96.00	7378.0
97.00	261.0
103.90	461.0
105.00	176.0
105.90	446.0
106.70	121.0
107.90	139.0
112.80	154.0
114.80	115.0
115.90	448.0
116.90	1030.0
117.90	433.0
118.90	810.0
127.90	408.0
128.90	206.0
129.80	458.0
130.80	142.0
134.70	170.0
136.90	239.0
139.90	126.0
140.90	1118.0
141.80	211.0
142.90	1970.0
144.00	201.0
144.90	952.0
145.80	154.0
147.80	275.0
149.80	155.0
153.00	126.0
154.80	308.0
157.00	169.0
158.80	119.0
160.90	136.0
170.80	449.0
171.90	2133.0
173.00	1682.0
173.90	100752.0
174.90	7569.0
175.90	98968.0
176.90	6536.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

177.80

196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328