

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062518\
 Data File : VV006431.D
 Acq On : 25 Jun 2018 15:05
 Operator : SY/MD
 Sample : VV0625WBL01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK62

Quant Time: Jun 26 07:00:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 26 06:50:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	338120	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	304191	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	133755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	101743	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.58	69	83043	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.80%
11) 1,1-Dichloroethene-d2	2.13	63	136967	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.97	46	146085	35.07	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	70.14%
24) Chloroform-d	4.41	84	162824	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
26) 1,2-Dichloroethane-d4	5.09	65	81866	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	5.10	84	369861	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.12	67	109524	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.36	98	344263	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.67	79	36249	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.14	63	142109	41.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59628	4.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	118746	4.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.60%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	11595	0.48 ug/L	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062518\
Data File : VV006431.D
Acq On : 25 Jun 2018 15:05
Operator : SY/MD
Sample : VV0625WBL01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK62

Quant Time: Jun 26 07:00:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 26 06:50:47 2018
Response via : Initial Calibration

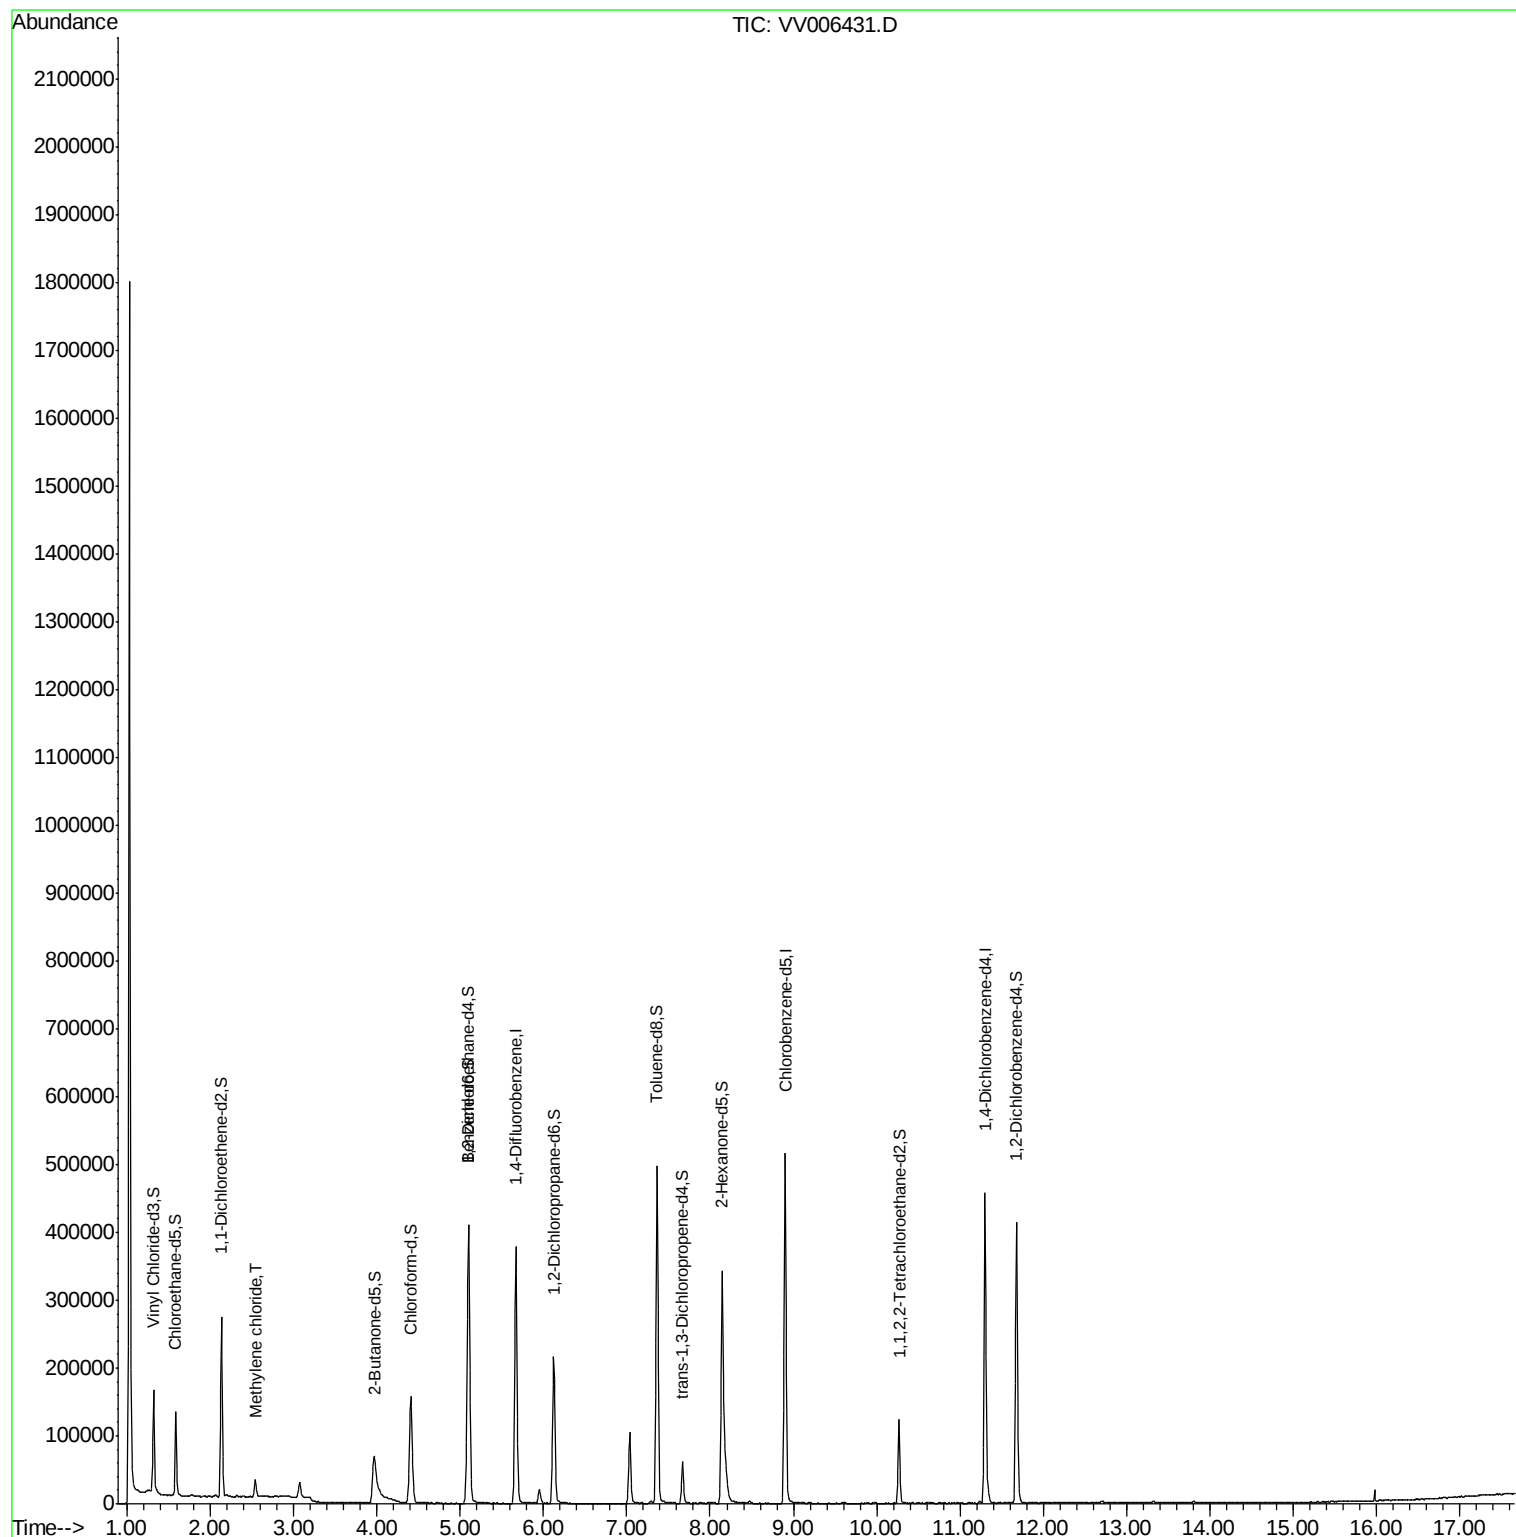

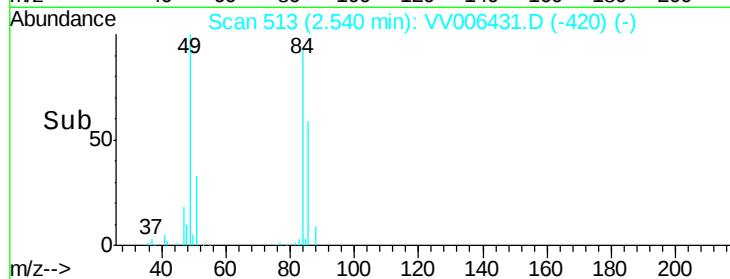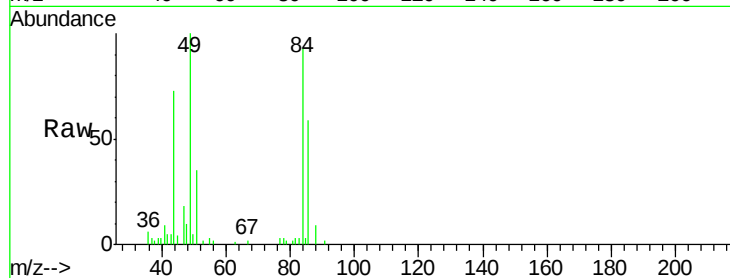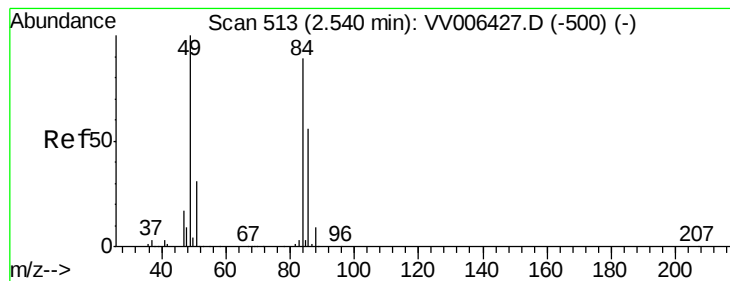

#16
Methylene chloride
Concen: 0.48 ug/L
RT: 2.54 min Scan# 513
Delta R.T. -0.00 min
Lab File: VV006431.D
Acq: 25 Jun 2018 15:05

Instrument :
MSVOA_V
ClientSampleId :
VBLK62

Tot Ion: 84 Resp: 11595

Ion	Ratio	Lower	Upper
84	100		
86	63.9	44.2	82.2
49	107.4	79.0	146.8

