

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062518\
 Data File : VV006447.D
 Acq On : 26 Jun 2018 00:19
 Operator : SY/MD
 Sample : J3673-16 40X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DAZA9

Quant Time: Jun 26 09:32:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 26 06:50:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	312849	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	282117	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	121800	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	95172	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	1.59	69	76212	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.00%
11) 1,1-Dichloroethene-d2	2.13	63	127200	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.97	46	185911	48.23	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.46%
24) Chloroform-d	4.41	84	161265	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.09	65	79989	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.11	84	358002	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.12	67	105815	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.37	98	321799	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.67	79	31424	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
46) 2-Hexanone-d5	8.14	63	138198	43.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.54%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	58851	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	112660	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
34) Trichloroethene	5.97	95	9192	0.39 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062518\
Data File : VV006447.D
Acq On : 26 Jun 2018 00:19
Operator : SY/MD
Sample : J3673-16 40X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DAZA9

Quant Time: Jun 26 09:32:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 26 06:50:47 2018
Response via : Initial Calibration

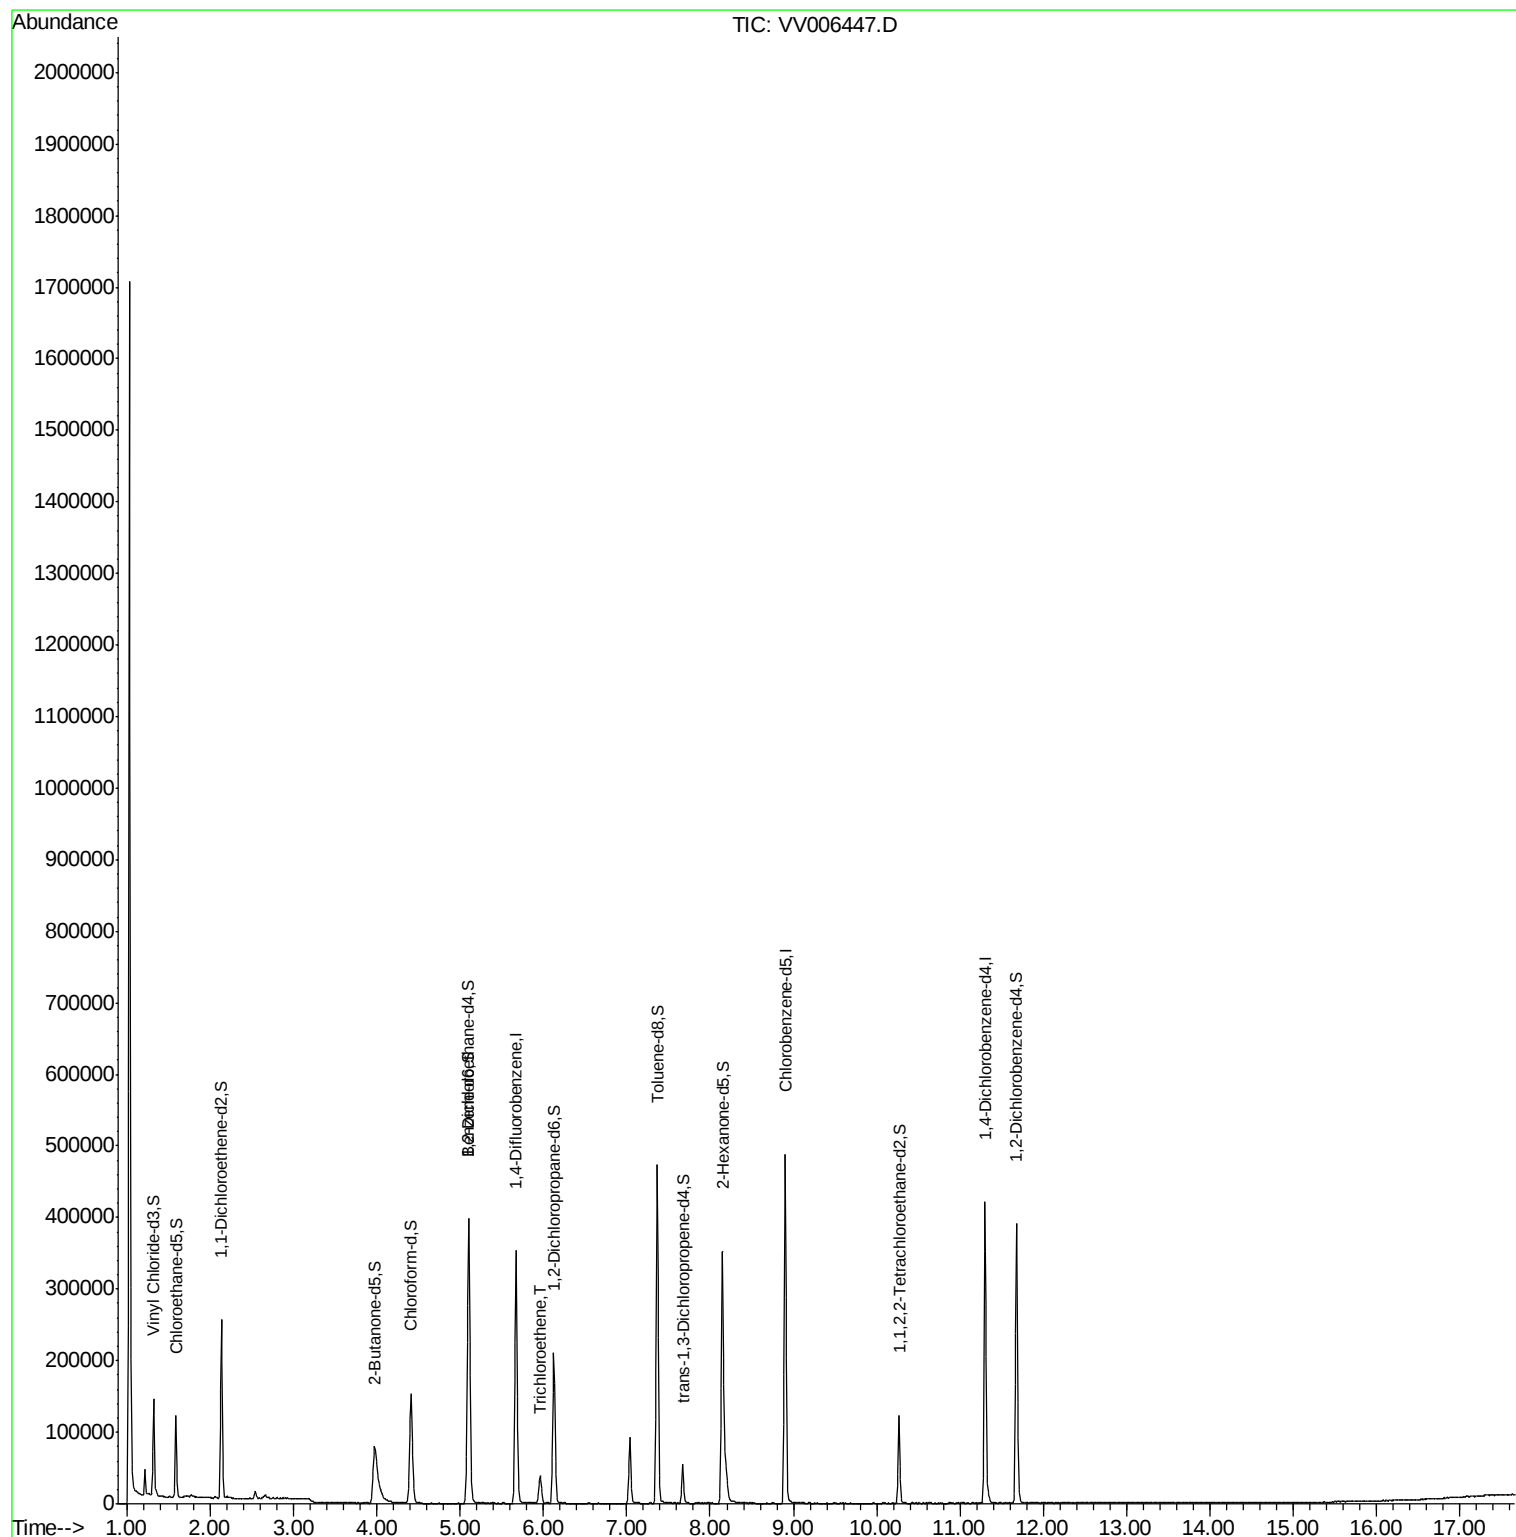

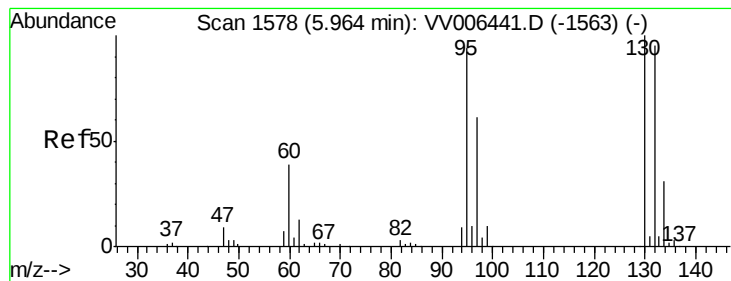

#34
 Trichloroethene
 Concen: 0.39 ug/L
 RT: 5.97 min Scan# 1579
 Delta R.T. 0.00 min
 Lab File: VV006447.D
 Acq: 26 Jun 2018 00:19

Instrument :
 MSVOA_V
 ClientSampleId :
 DAZA9

Tot Ion:	95	Resp:	9192
Ion	Ratio	Lower	Upper
95	100		
97	65.3	44.6	82.8
132	99.6	70.1	130.1
130	106.3	73.3	136.1

