

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062518\
 Data File : VV006451.D
 Acq On : 26 Jun 2018 02:06
 Operator : SY/MD
 Sample : J3674-13DL 100X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DAZC7DL

Quant Time: Jun 26 09:33:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 26 06:50:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	313075	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	280334	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	115313	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	89919	4.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.40%
7) Chloroethane-d5	1.58	69	74878	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.13	63	117768	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	3.96	46	186265	48.29	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.58%
24) Chloroform-d	4.41	84	151599	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	5.09	65	78462	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.11	84	339273	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.12	67	102365	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.37	98	298485	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	7.67	79	29132	3.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.80%
46) 2-Hexanone-d5	8.14	63	137078	43.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.38%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	57744	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	103861	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.97	96	6765	0.30 ug/L	91
34) Trichloroethene	5.96	95	72754	3.07 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062518\
Data File : VV006451.D
Acq On : 26 Jun 2018 02:06
Operator : SY/MD
Sample : J3674-13DL 100X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DAZC7DL

Quant Time: Jun 26 09:33:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 26 06:50:47 2018
Response via : Initial Calibration

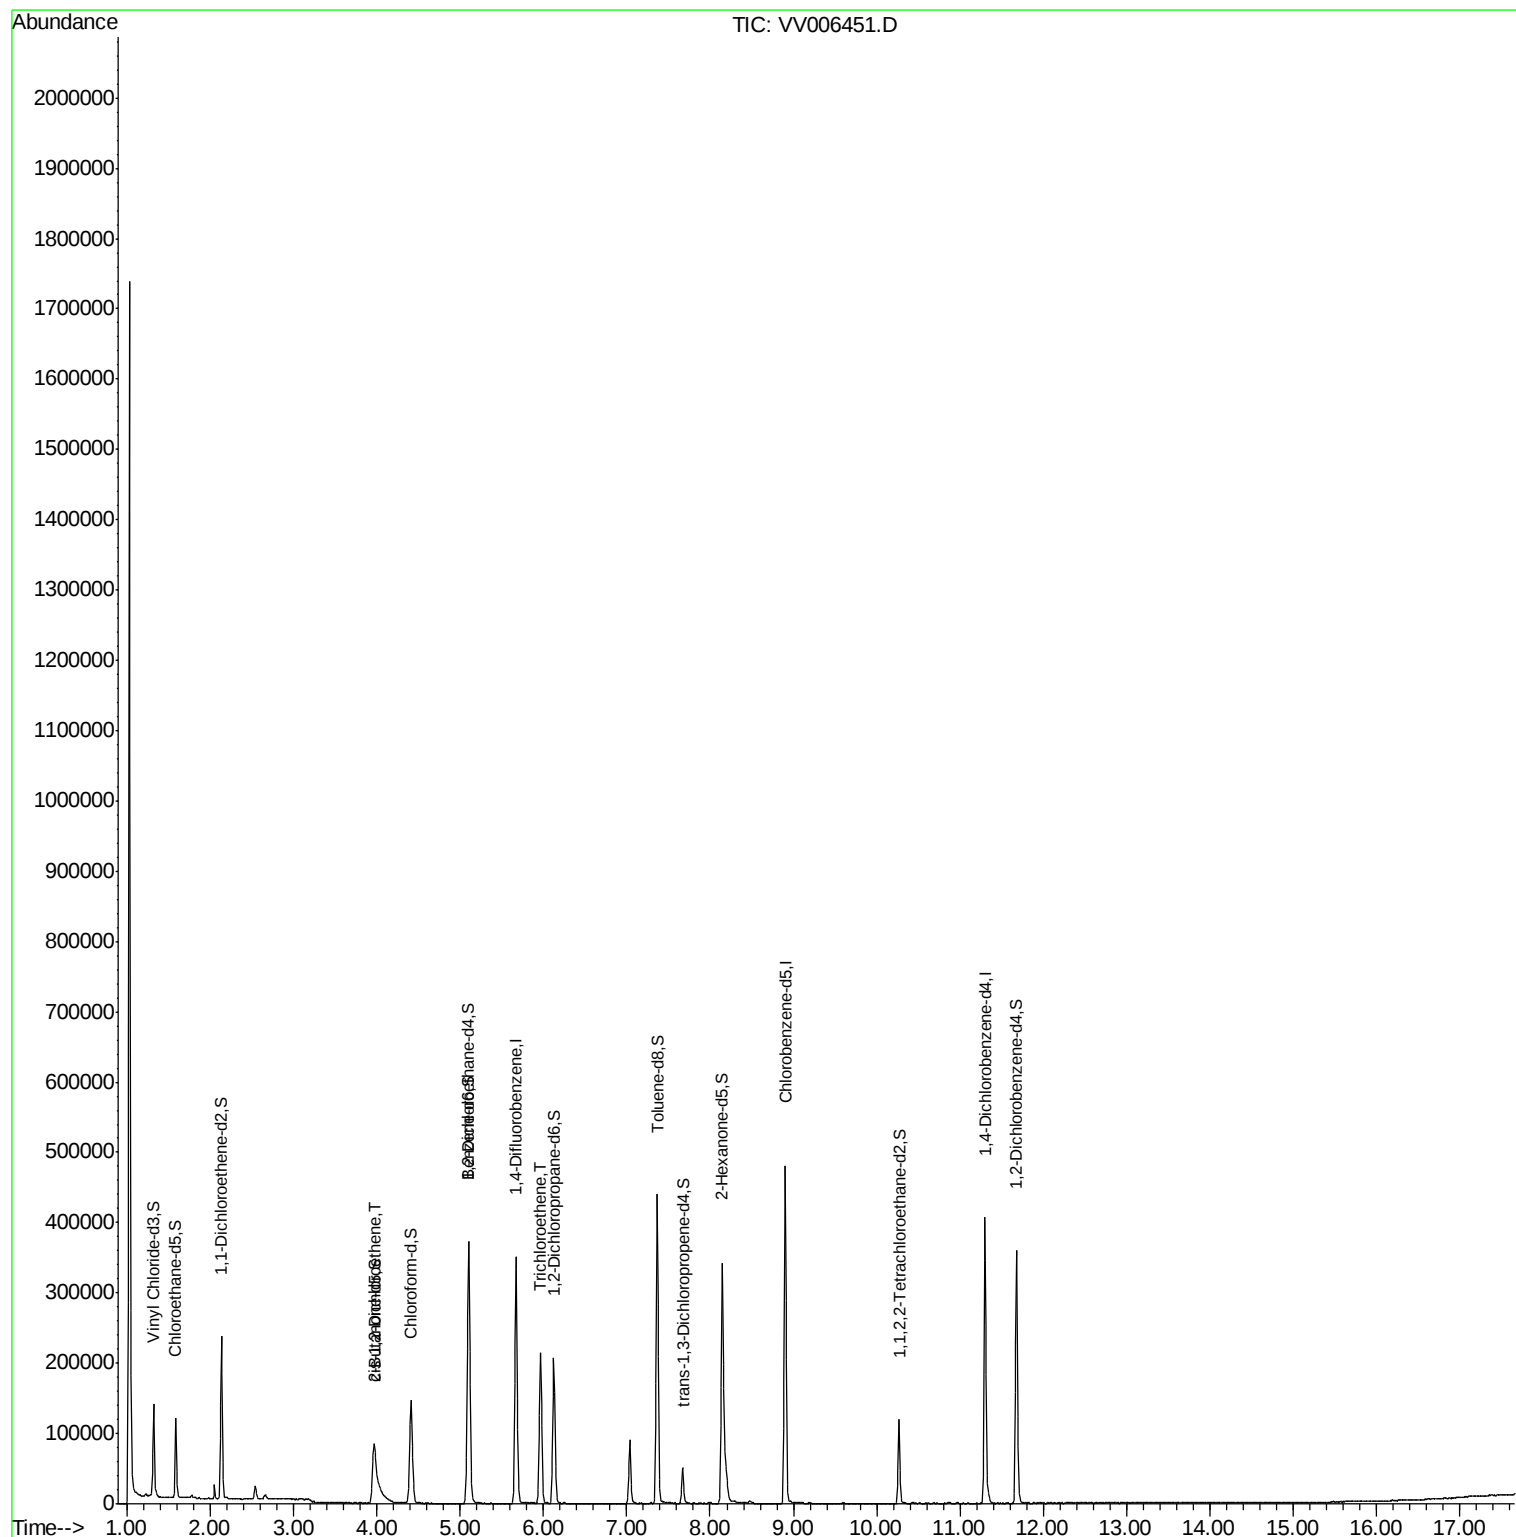

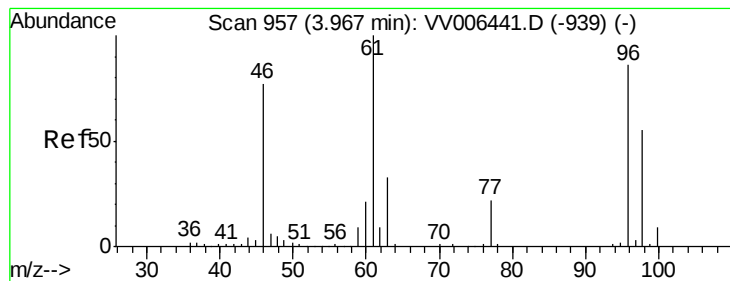

#22

cis-1,2-Dichloroethene

Concen: 0.30 ug/L

RT: 3.97 min Scan# 958

Delta R.T. -0.00 min

Lab File: VV006451.D

Acq: 26 Jun 2018 02:06

Instrument :

MSVOA_V

ClientSampleId :

DAZC7DL


Tot Ion: 96 Resp: 6765

Ion Ratio Lower Upper

96 100

61 126.8 81.8 151.8




68 0.0 0.0 0.0

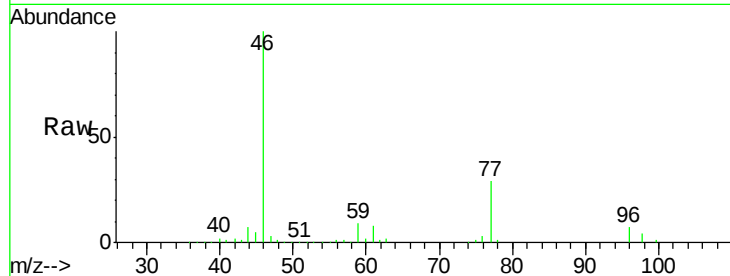

Abundance Ion 96.00 (95.70 to 96.70): VV006441.D (-939) (-)

Ion 61.05 (60.75 to 61.75): VV006441.D (-939) (-)

Ion 68.15 (67.85 to 68.85): VV006441.D (-939) (-)

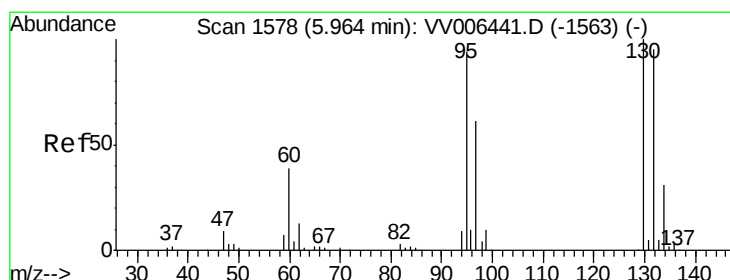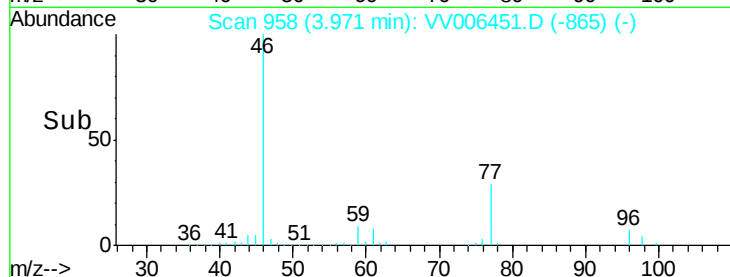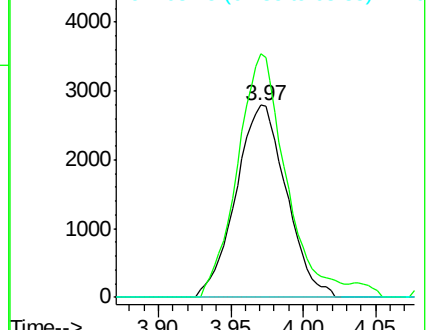

#34

Trichloroethene

Concen: 3.07 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV006451.D

Acq: 26 Jun 2018 02:06

Tgt Ion: 95 Resp: 72754


Ion Ratio Lower Upper

95 100

97 63.9 44.6 82.8

132 99.4 70.1 130.1

130 106.1 73.3 136.1

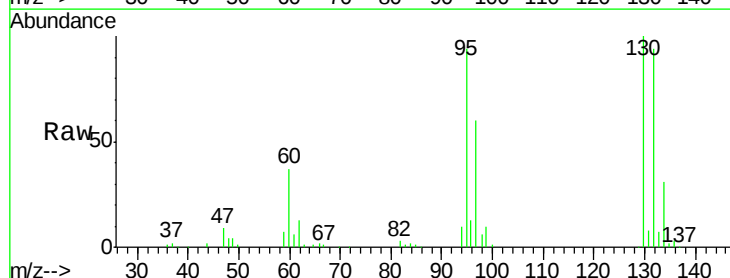

Abundance Ion 95.00 (94.70 to 95.70): VV006441.D (-1563) (-)

Ion 96.95 (96.65 to 97.65): VV006441.D (-1563) (-)

Ion 131.95 (131.65 to 132.65): VV006441.D (-1563) (-)

Ion 129.95 (129.65 to 130.65): VV006441.D (-1563) (-)

