


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062518\
 Data File : VV006424.D
 Acq On : 25 Jun 2018 09:33
 Operator : SY/MD
 Sample : BFB79
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 27 02:22:39 2018

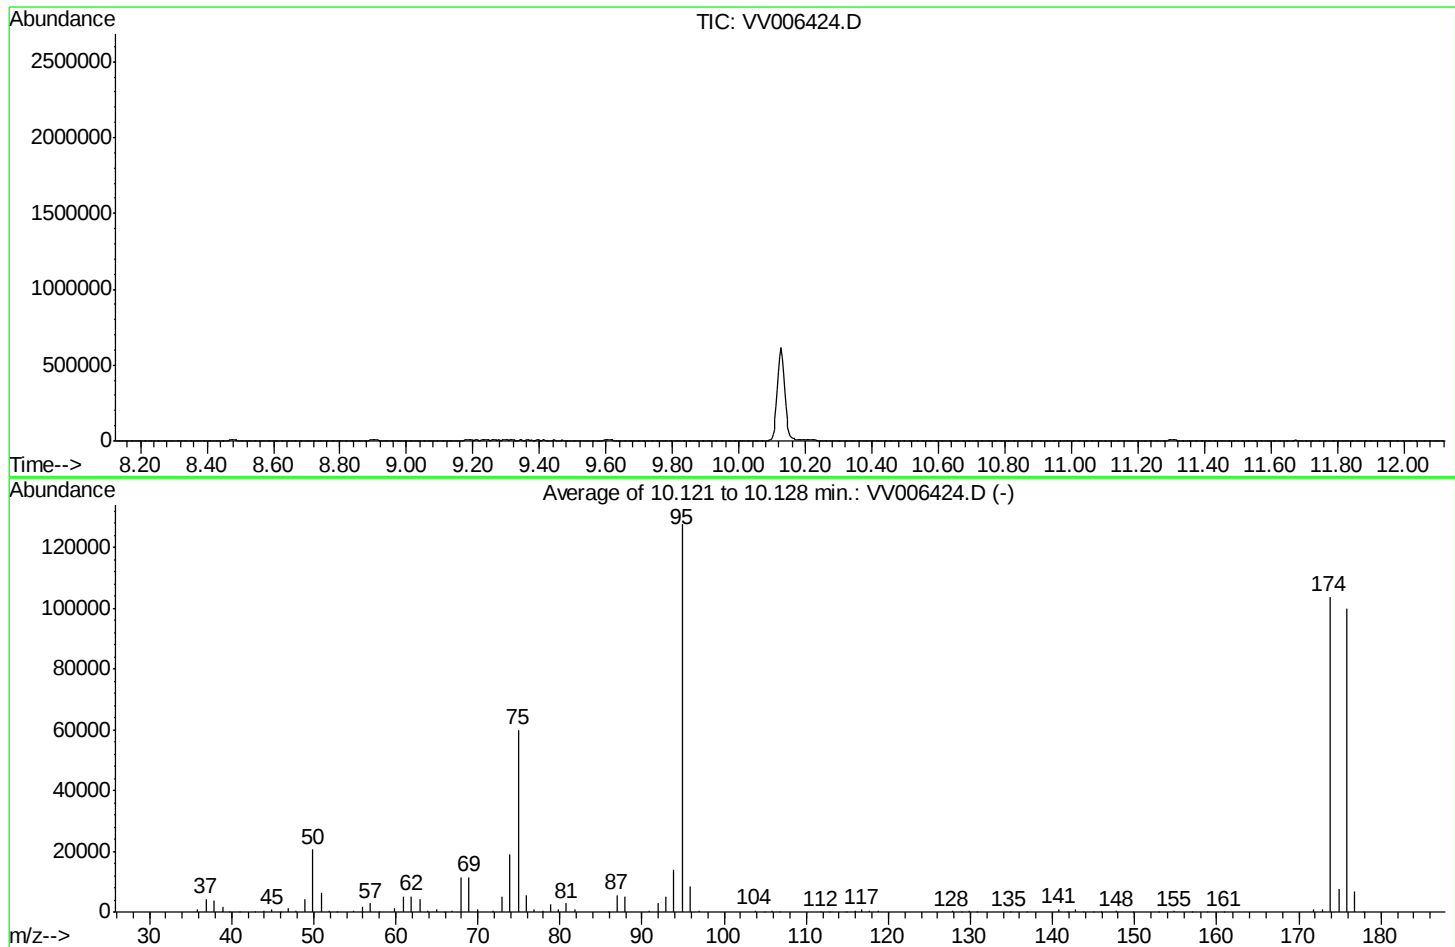

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	20496	PASS
75	95	30	80	46.9	59824	PASS
95	95	100	100	100.0	127544	PASS
96	95	5	9	6.8	8629	PASS
173	174	0.00	2	0.7	720	PASS
174	95	50	120	81.4	103802	PASS
175	174	5	9	7.3	7620	PASS
176	174	95	101	96.0	99685	PASS
177	176	5	9	6.6	6594	PASS

Scan 2858 (10.080 min): VV006424.D
BFB79

m/z	Abundance
35.80	1273.0
36.80	123.0
37.80	492.0
38.90	132.0
39.70	220.0
43.90	624.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	1883.0
36.90	4189.0
37.90	4368.0
38.90	1720.0
39.80	273.0
40.90	154.0
42.80	162.0
43.90	1091.0
44.90	884.0
45.90	111.0
46.90	1294.0
47.90	570.0
48.90	4133.0
49.90	19576.0
50.90	6289.0
51.80	307.0
52.90	115.0
54.80	321.0
55.90	1446.0
56.90	2764.0
58.00	126.0
59.90	989.0
60.90	4930.0
61.90	4879.0
62.90	3924.0
64.00	505.0
64.90	621.0
65.90	104.0
66.90	354.0
67.90	10921.0
68.90	11066.0
69.90	921.0
71.90	548.0
72.90	4831.0
73.90	18248.0
74.90	57168.0
75.90	5205.0
76.90	682.0
77.90	551.0
78.80	2599.0
79.80	818.0
80.80	2622.0
81.80	714.0
85.80	196.0
86.90	5533.0
87.90	4928.0
90.90	374.0
91.90	2888.0
92.90	4993.0
93.90	13145.0
94.90	120160.0
95.90	8223.0
96.90	286.0
103.80	457.0
104.90	145.0
105.80	451.0
106.70	103.0
111.80	137.0
114.80	179.0
115.90	336.0
116.80	626.0
117.70	343.0
118.80	621.0
127.80	437.0
128.80	182.0
129.80	349.0
130.90	114.0
134.80	164.0
136.80	154.0
140.80	953.0
141.90	132.0
142.80	1017.0
144.90	139.0
145.90	120.0
147.90	275.0
149.80	158.0
152.80	119.0
154.80	325.0
156.90	156.0
158.90	137.0
171.80	992.0
173.00	680.0
173.80	95312.0
174.90	7224.0
175.80	91496.0
176.90	6226.0
177.80	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	2072.0
36.90	4545.0
37.90	4663.0
38.90	1935.0
39.90	289.0
40.90	163.0
42.80	152.0
43.90	1080.0
44.90	842.0
45.90	132.0
46.90	1432.0
47.90	580.0
48.90	4516.0
49.90	21144.0
50.90	6766.0
51.80	315.0
52.80	121.0
54.80	363.0
55.90	1624.0
56.90	3057.0
58.00	136.0
59.90	1149.0
60.90	5353.0
61.90	5354.0
62.90	4217.0
64.00	578.0
64.90	664.0
66.90	378.0
67.90	11917.0
68.90	11861.0
69.90	988.0
71.90	587.0
72.90	5105.0
73.90	19736.0
74.90	61872.0
75.90	5698.0
76.90	777.0
77.80	541.0
78.80	2798.0
79.90	885.0
80.80	2860.0
81.80	728.0
85.90	227.0
86.90	5815.0
87.90	5215.0
90.80	389.0
91.90	3215.0
92.90	5479.0
93.90	14449.0
94.90	132224.0
95.90	8948.0
97.00	335.0
103.80	466.0
104.80	173.0
105.80	444.0
111.80	125.0
112.80	106.0
114.80	162.0
115.90	344.0
116.80	708.0
117.80	380.0
118.80	613.0
127.80	405.0
128.80	216.0
129.80	369.0
130.80	134.0
134.80	212.0
136.80	189.0
140.80	1046.0
141.80	147.0
142.80	1033.0
143.70	103.0
144.90	147.0
145.80	128.0
147.80	277.0
149.80	171.0
152.90	138.0
154.80	373.0
157.00	186.0
158.80	140.0
171.80	1060.0
172.90	723.0
173.80	107216.0
174.90	7870.0
175.80	102968.0
176.90	6810.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	2216.0
36.90	4390.0
37.90	4485.0
38.90	1983.0
39.90	298.0
40.90	155.0
42.80	143.0
43.90	1051.0
44.90	773.0
45.90	129.0
46.90	1372.0
47.80	588.0
48.90	4445.0
49.90	20768.0
50.90	6481.0
51.90	285.0
52.80	148.0
54.80	359.0
55.90	1648.0
56.90	3026.0
57.90	140.0
59.80	1119.0
60.90	5198.0
61.90	5363.0
62.90	4064.0
63.90	573.0
65.00	698.0
66.90	366.0
67.90	11492.0
68.90	11617.0
69.90	957.0
71.90	582.0
72.90	4904.0
73.90	19240.0
74.90	60432.0
75.90	5501.0
76.90	788.0
77.80	514.0
78.80	2718.0
79.90	931.0
80.80	2824.0
81.80	711.0
85.90	223.0
86.90	5492.0
87.90	5134.0
90.80	385.0
91.90	3256.0
92.90	5261.0
93.90	14355.0
94.90	130248.0
95.90	8716.0
96.90	330.0
103.70	466.0
104.80	193.0
105.80	424.0
112.80	109.0
114.80	123.0
115.90	325.0
116.80	715.0
117.80	383.0
118.80	529.0
127.80	363.0
128.90	219.0
129.80	371.0
130.80	146.0
134.80	208.0
136.80	204.0
140.80	1037.0
141.80	120.0
142.80	983.0
144.90	152.0
145.80	143.0
147.80	266.0
149.80	152.0
152.90	136.0
154.90	374.0
157.00	182.0
158.80	115.0
160.90	103.0
171.90	1014.0
172.80	758.0
173.80	108880.0
174.90	7768.0
175.80	104592.0
176.80	6746.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79