


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062519\
Data File : VV011743.D
Acq On : 25 Jun 2019 08:41
Operator : SY/MD
Sample : BFB56
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Jun 26 01:40:21 2019

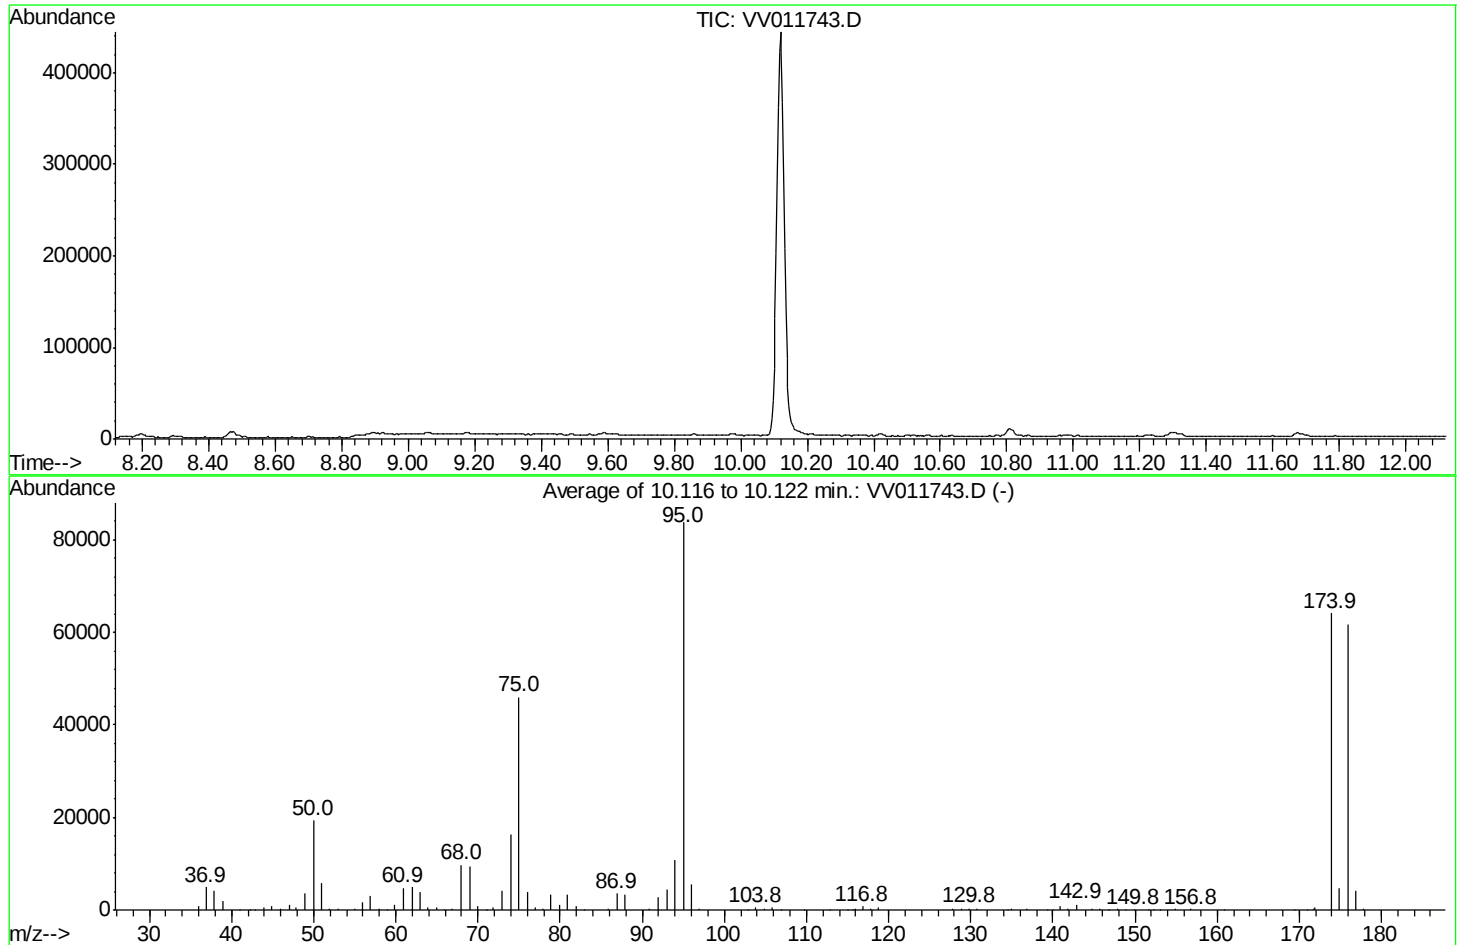

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	19240	PASS
75	95	30	80	54.9	45978	PASS
95	95	100	100	100.0	83789	PASS
96	95	5	9	6.5	5445	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.5	64096	PASS
175	174	5	9	7.2	4638	PASS
176	174	95	101	96.4	61776	PASS
177	176	5	9	6.6	4063	PASS

Scan 2793 (10.071 min): VV011743.D
BFB56

m/z	Abundance
35.90	1623.0
36.90	207.0
37.90	733.0
38.70	150.0
39.80	439.0
43.10	189.0
43.90	515.0
45.00	104.0
48.80	109.0
67.40	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.90	2521.0
36.90	5151.0
37.90	4996.0
39.00	1959.0
39.90	384.0
40.90	123.0
42.20	100.0
42.80	132.0
44.00	1102.0
44.90	950.0
45.90	153.0
47.00	1077.0
47.90	645.0
49.00	3980.0
50.00	18920.0
51.00	5955.0
51.90	320.0
53.00	175.0
55.10	326.0
55.90	1788.0
56.90	3155.0
57.90	161.0
58.90	118.0
59.90	1036.0
60.90	4724.0
62.00	4917.0
63.00	3723.0
63.90	517.0
65.00	646.0
65.90	131.0
66.90	321.0
68.00	9576.0
69.00	9453.0
70.00	793.0
71.90	554.0
72.90	4268.0
74.00	16234.0
75.00	45656.0
76.00	4079.0
77.00	503.0
77.90	333.0
78.90	3155.0
79.90	1041.0
80.80	3397.0
81.90	931.0
83.00	133.0
85.90	159.0
86.90	3385.0
87.90	3417.0
90.80	349.0
92.00	2775.0
92.90	4158.0
93.90	10555.0
95.00	81848.0
96.00	5512.0
96.90	177.0
102.90	104.0
103.90	400.0
104.80	152.0
105.70	406.0
106.90	113.0
109.80	122.0
112.80	113.0
115.00	131.0
115.60	283.0
116.00	318.0
116.80	727.0
117.90	330.0
118.80	543.0
127.70	325.0
129.00	219.0
129.80	335.0
130.70	162.0
134.50	124.0
135.00	174.0
136.80	176.0
139.90	125.0
140.80	907.0
141.80	200.0
142.90	1109.0
144.70	146.0
145.80	167.0
146.80	108.0
147.80	256.0
152.20	152.0
153.00	122.0
154.90	177.0
156.80	178.0
169.50	122.0
171.70	587.0
172.00	581.0
173.90	61424.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

174.90	4627.0
175.90	59256.0
176.90	4045.0
177.80	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.90	2630.0
36.90	5252.0
38.00	4972.0
39.00	2047.0
40.00	347.0
40.90	123.0
42.20	107.0
42.80	122.0
44.10	1100.0
44.90	976.0
45.90	170.0
47.00	1168.0
47.80	712.0
49.00	3840.0
50.00	20072.0
51.00	6071.0
51.90	344.0
53.00	181.0
55.00	275.0
55.90	1839.0
56.90	3179.0
57.90	161.0
59.00	141.0
59.90	1067.0
60.90	5024.0
62.00	5043.0
63.00	3963.0
63.90	563.0
65.00	611.0
65.90	150.0
66.90	324.0
68.00	10083.0
69.00	9693.0
70.00	908.0
71.90	642.0
72.90	4232.0
74.00	16960.0
75.00	47600.0
76.00	4049.0
77.00	496.0
77.90	356.0
78.90	3452.0
79.90	1008.0
80.80	3525.0
81.90	900.0
82.90	122.0
85.90	163.0
86.90	3670.0
87.90	3515.0
90.80	379.0
91.90	2916.0
93.00	4589.0
93.90	11130.0
95.00	86640.0
96.00	5583.0
96.90	186.0
102.80	105.0
103.80	471.0
104.80	187.0
105.70	429.0
106.80	105.0
109.80	124.0
112.70	122.0
115.00	149.0
116.00	381.0
116.90	769.0
117.90	357.0
118.80	575.0
127.80	307.0
128.90	170.0
129.80	339.0
130.70	172.0
135.00	190.0
136.80	158.0
139.90	126.0
140.90	929.0
141.80	193.0
142.90	1155.0
144.70	191.0
145.70	159.0
146.80	108.0
147.90	241.0
148.90	105.0
149.80	122.0
151.70	107.0
152.30	118.0
153.00	134.0
155.00	189.0
156.80	205.0
160.80	104.0
169.40	104.0
171.90	660.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

173.90	66000.0
174.90	4816.0
175.90	64080.0
176.90	4158.0
177.80	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.90	2529.0
37.00	4866.0
38.00	4783.0
39.00	1880.0
39.90	320.0
40.90	121.0
42.30	124.0
42.80	112.0
44.00	1033.0
44.90	927.0
45.90	178.0
47.00	1097.0
47.80	672.0
49.00	3601.0
50.00	18728.0
51.00	5555.0
51.90	317.0
52.90	160.0
54.90	265.0
55.90	1705.0
56.90	2977.0
58.00	147.0
59.00	132.0
59.90	966.0
60.90	4702.0
62.00	4796.0
63.00	3859.0
63.90	513.0
65.00	519.0
66.00	125.0
66.90	338.0
67.90	9412.0
69.00	9117.0
70.00	877.0
71.00	110.0
71.90	649.0
73.00	3807.0
74.00	16090.0
75.00	44680.0
76.00	3722.0
77.00	482.0
78.00	290.0
78.90	3254.0
79.90	894.0
80.90	3318.0
81.90	742.0
82.80	118.0
85.90	144.0
86.90	3429.0
87.90	3175.0
90.80	364.0
91.90	2858.0
93.00	4466.0
93.90	10537.0
95.00	82880.0
96.00	5240.0
97.00	145.0
102.70	111.0
103.80	462.0
104.80	188.0
105.80	438.0
109.70	106.0
112.70	124.0
114.90	132.0
116.00	370.0
116.90	739.0
117.80	409.0
118.80	531.0
127.80	328.0
128.80	131.0
129.90	311.0
130.70	181.0
135.00	196.0
136.70	159.0
139.30	105.0
139.90	106.0
140.90	910.0
141.80	166.0
142.90	1112.0
144.80	202.0
145.70	146.0
147.90	223.0
149.90	123.0
151.70	110.0
153.10	111.0
154.90	225.0
156.80	221.0
160.80	136.0
170.90	126.0
171.90	715.0
173.90	64864.0
174.90	4473.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

175.90	61992.0
176.90	3988.0
177.80	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56