

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017124.D
 Acq On : 25 Jun 2020 13:59
 Operator : SY/MD
 Sample : L3105-05DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXK8DL

Quant Time: Jun 26 01:34:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 01:31:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	175102	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	169458	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	79007	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	54724	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	42571	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.40%
11) 1,1-Dichloroethene-d2	2.12	63	80256	4.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.20%
20) 2-Butanone-d5	3.95	46	133908	50.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.00%
24) Chloroform-d	4.38	84	116415	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
26) 1,2-Dichloroethane-d4	5.06	65	63122	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.08	84	219587	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.10	67	64048	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.34	98	189117	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
45) trans-1,3-Dichloropropene-	7.64	79	25466	4.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.00%
48) 2-Hexanone-d5	8.11	63	94256	45.13	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.26%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	44081	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	74312	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.32	62	117389	10.217	ug/L	97
8) Chloroethane	1.32	64	38221	6.019	ug/L #	48
10) 1,1,2-Trichloro-1,2,2-trif	2.12	101	1012	0.109	ug/L #	23
12) 1,1-Dichloroethene	2.13	96	3550	0.422	ug/L #	1
15) Methyl Acetate	2.51	43	2184	0.660	ug/L #	61
16) Methylene chloride	2.53	84	1712	0.190	ug/L	89
18) trans-1,2-Dichloroethene	2.78	96	2288	0.257	ug/L	98
19) 1,1-Dichloroethane	3.21	63	59406	2.969	ug/L	98
21) 2-Butanone	4.12	43	76145	29.834	ug/L #	50
22) cis-1,2-Dichloroethene	3.94	96	64521	5.298	ug/L	94
25) Chloroform	4.40	83	4027	0.184	ug/L	83
27) 1,2-Dichloroethane	5.16	62	1914	0.141	ug/L #	88
29) 1,1,1-Trichloroethane	4.63	97	16555	0.815	ug/L	96
30) Cyclohexane	4.69	56	7624	0.395	ug/L	96
31) Carbon tetrachloride	4.64	117	1982	0.108	ug/L	87
33) Benzene	5.13	78	14223	0.320	ug/L	100
34) Trichloroethene	5.94	95	1588	0.122	ug/L	88

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017124.D
 Acq On : 25 Jun 2020 13:59
 Operator : SY/MD
 Sample : L3105-05DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXK8DL

Quant Time: Jun 26 01:34:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 01:31:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) Methylcyclohexane	6.10	83	16997	0.841	ug/L #	18
37) 1,2-Dichloropropane	6.10	63	8409	0.765	ug/L #	85
39) cis-1,3-Dichloropropene	7.01	75	2076	0.127	ug/L #	40
43) 1,3,5-Trimethylbenzene	11.36	105	5692	0.123	ug/L	87
46) trans-1,3-Dichloropropene	7.64	75	1378	0.098	ug/L #	64
47) 1,1,2-Trichloroethane	7.87	97	2535	0.325	ug/L #	78
53) Chlorobenzene	8.90	112	45420	1.412	ug/L	95
56) o-xylene	9.56	106	3998	0.198	ug/L	98
63) 1,3-Dichlorobenzene	11.21	146	3474	0.146	ug/L #	85
64) 1,4-Dichlorobenzene	11.30	146	7319	0.303	ug/L	91
66) 1,2-Dichlorobenzene	11.67	146	3357	0.156	ug/L	93
70) Naphthalene	13.53	128	2935	0.132	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062520\
Data File : VV017124.D
Acq On : 25 Jun 2020 13:59
Operator : SY/MD
Sample : L3105-05DL 10X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXK8DL

Quant Time: Jun 26 01:34:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 01:31:34 2020
Response via : Initial Calibration

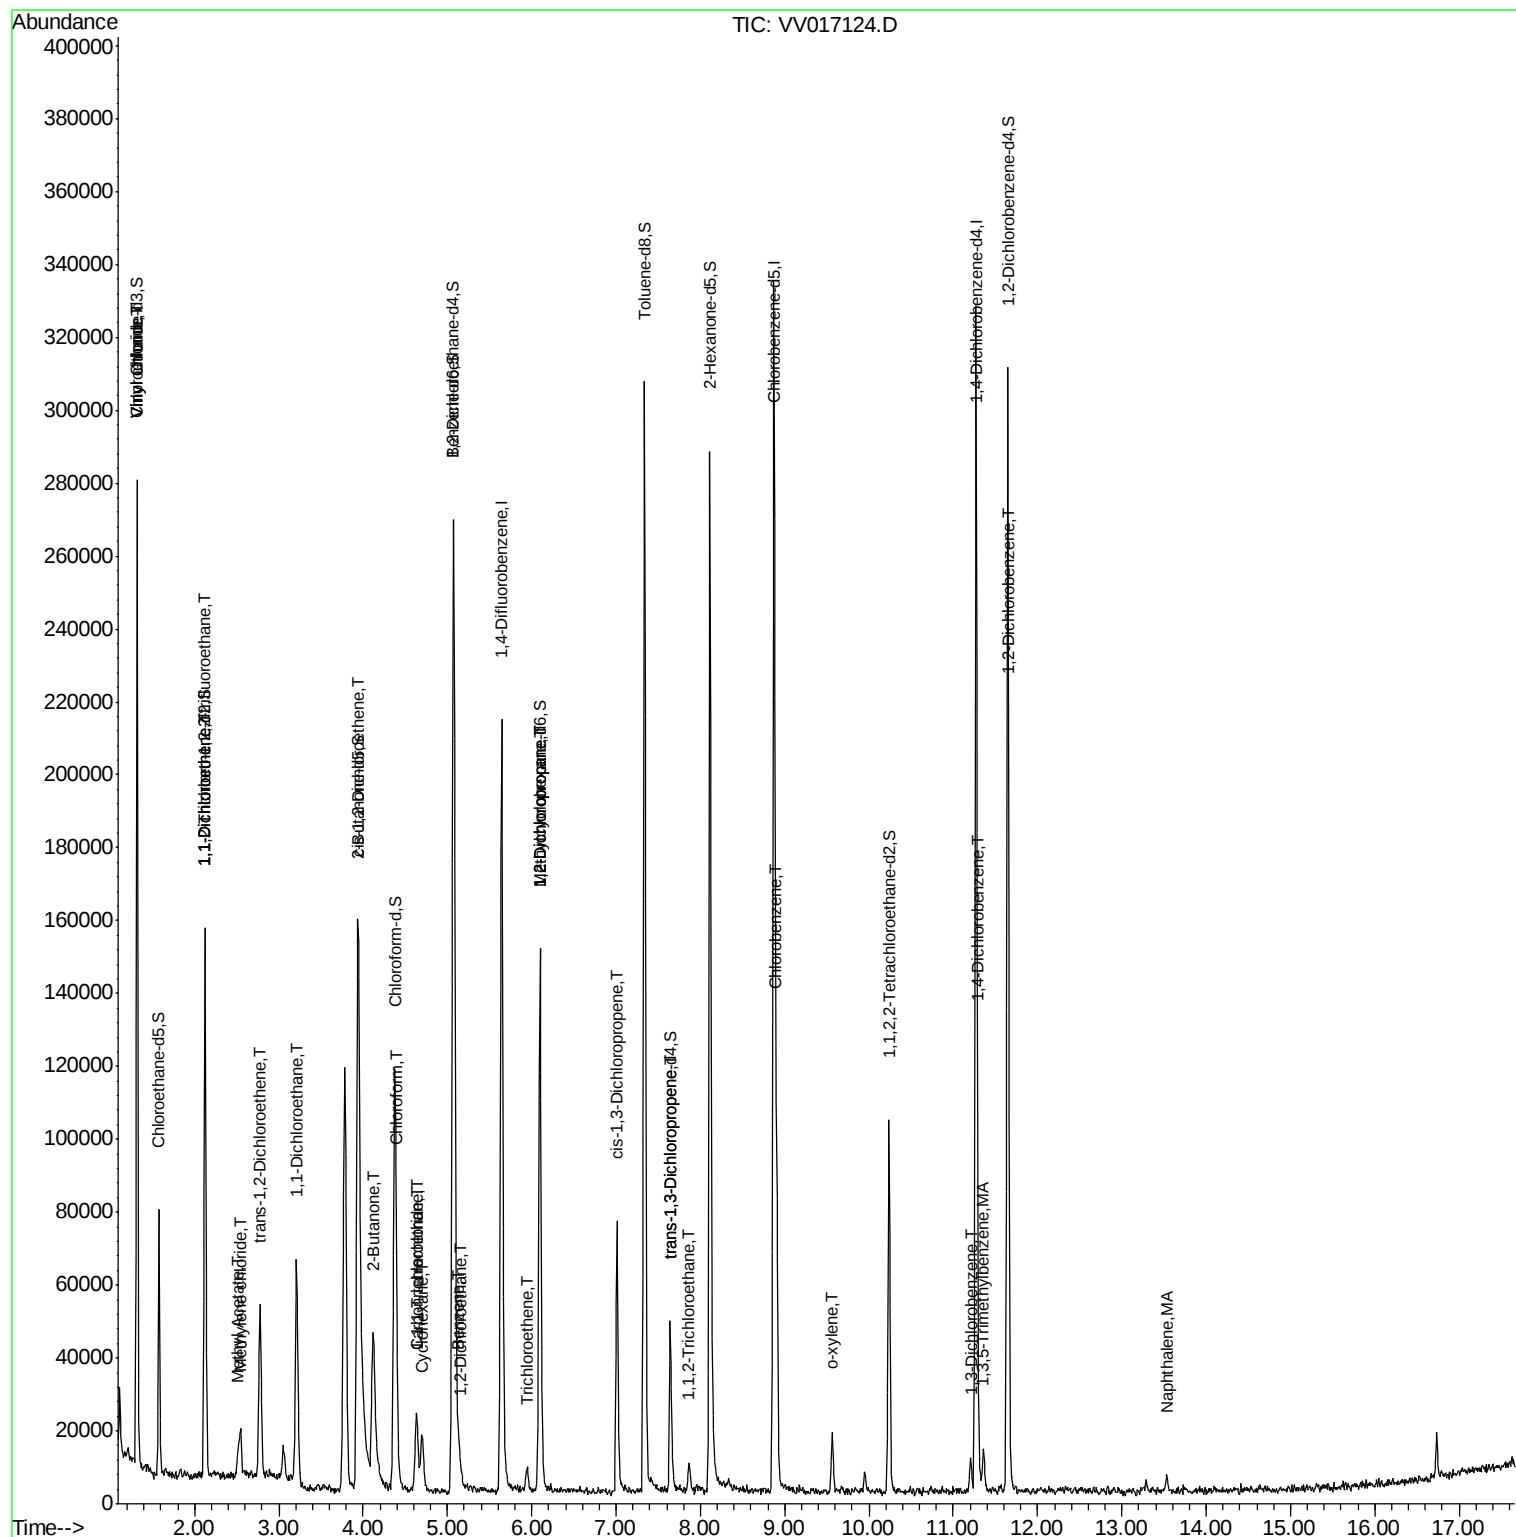



#5

Vinyl chloride

Concen: 10.217 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :





BFXK8DL

Tot Ion: 62 Resp: 117389

Ion Ratio Lower Upper

62 100

64 33.6 22.5 41.7

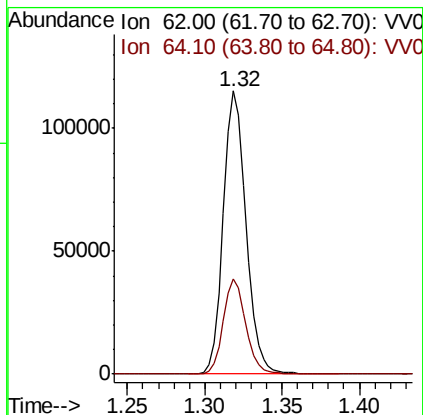

#8

Chloroethane

Concen: 6.019 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.28 min

Lab File: VV017124.D




Acq: 25 Jun 2020 13:59


Tgt Ion: 64 Resp: 38221

Ion Ratio Lower Upper

64 100

66 3.6 22.8 42.4#

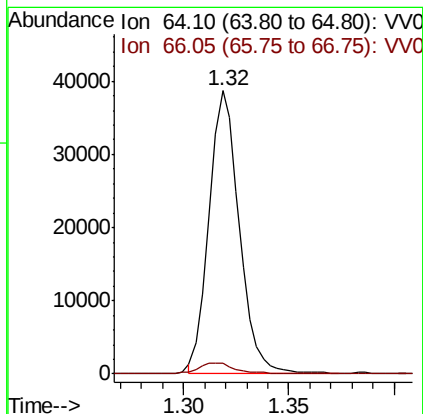



#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.109 ug/L

RT: 2.12 min Scan# 321

Delta R.T. -0.01 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :

BFXK8DL


Tot Ion:101 Resp: 1012

Ion Ratio Lower Upper

101 100

85 4.4 35.4 53.2#




151 4.2 63.9 95.9#

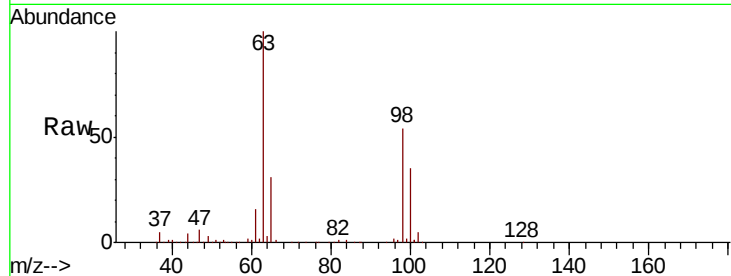

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VV0

Ion 151.00 (150.70 to 151.70): V

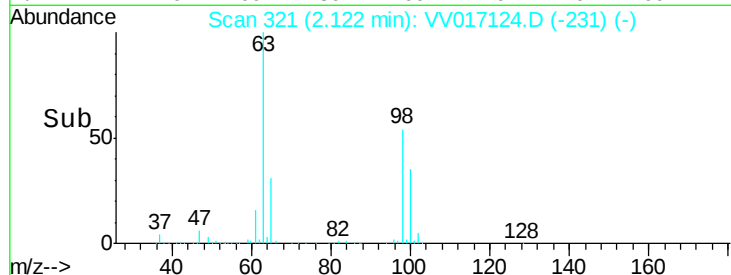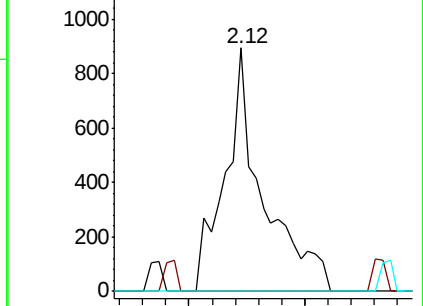

#12

1,1-Dichloroethene

Concen: 0.422 ug/L

RT: 2.13 min Scan# 324

Delta R.T. -0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59


Tgt Ion: 96 Resp: 3550

Ion Ratio Lower Upper

96 100

61 412.5 125.0 232.2#



63 1724.9 109.8 203.8#




Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 63.00 (62.70 to 63.70): VV0




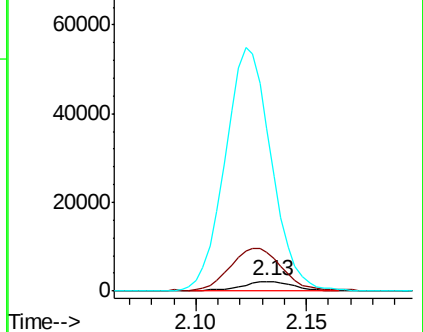


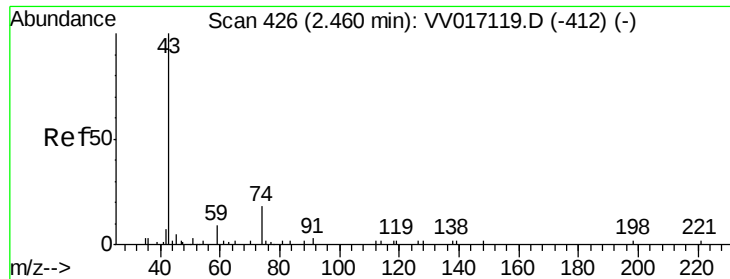

#15
Methvl Acetate
Concen: 0.660 ug/L
RT: 2.51 min Scan# 442
Delta R.T. 0.05 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59




Instrument :
MSVOA_V
ClientSampled :
BFXK8DL


Tot Ion: 43 Resp: 2184
Ion Ratio Lower Upper
43 100
74 4.5 19.1 28.7#

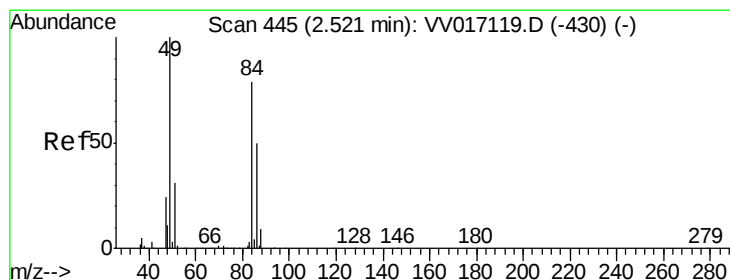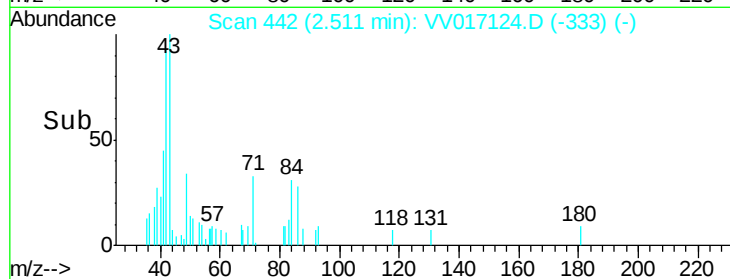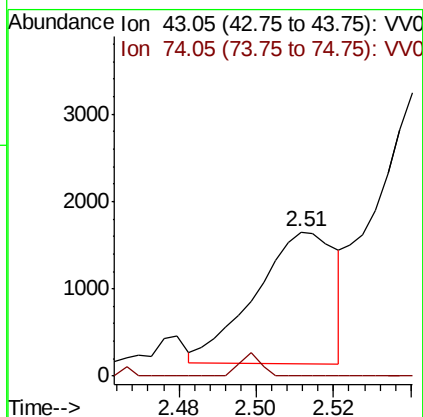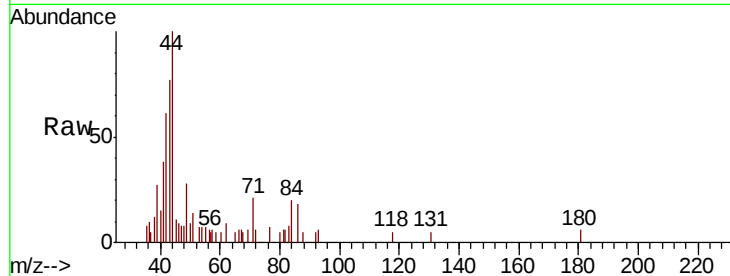

#16
Methylene chloride
Concen: 0.190 ug/L
RT: 2.53 min Scan# 447
Delta R.T. 0.01 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59

Tgt Ion: 84 Resp: 1712
Ion Ratio Lower Upper
84 100
86 57.2 45.8 85.0
49 141.4 89.6 166.4

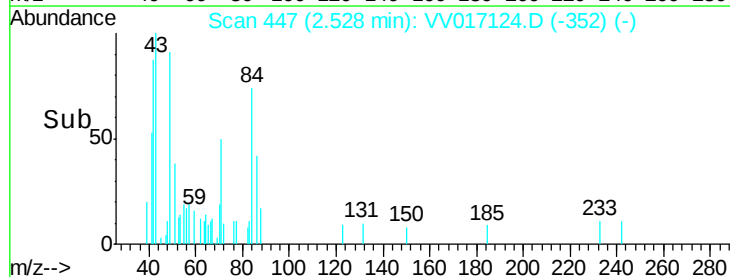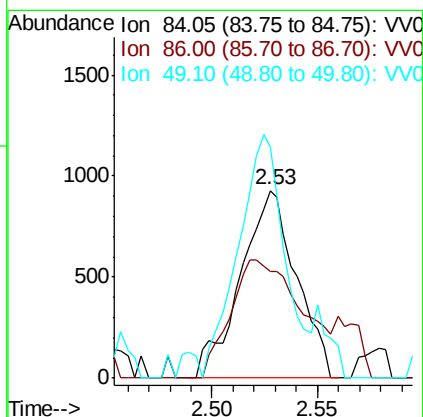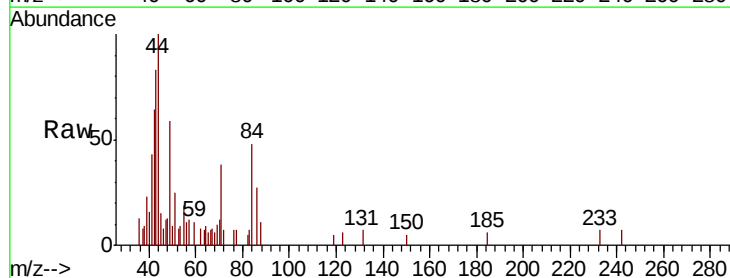

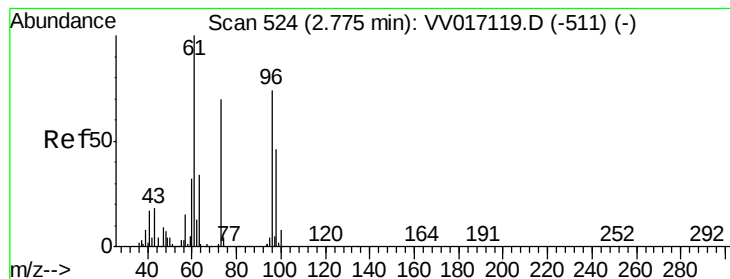

#18

trans-1,2-Dichloroethene

Concen: 0.257 ug/L

RT: 2.78 min Scan# 524

Delta R.T. -0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :

BFXK8DL





Tot Ion: 96 Resp: 2288

Ion Ratio Lower Upper

96 100

61 146.7 102.3 189.9

98 59.3 44.7 82.9

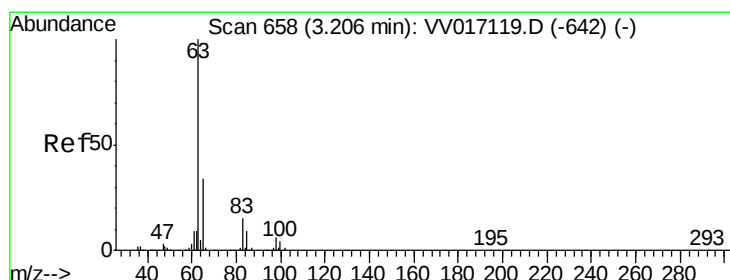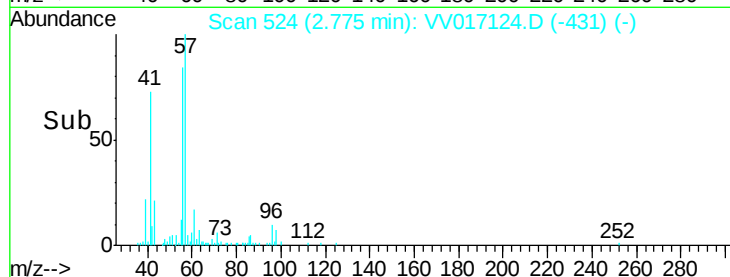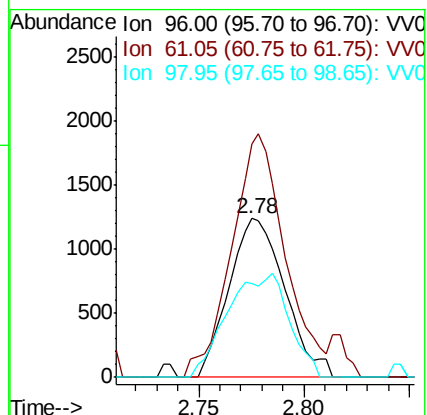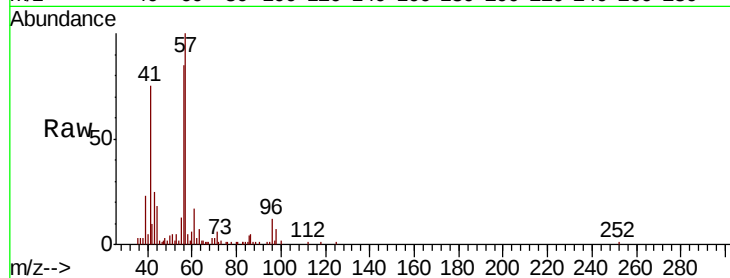

#19

1,1-Dichloroethane

Concen: 2.969 ug/L

RT: 3.21 min Scan# 659

Delta R.T. 0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59




Tgt Ion: 63 Resp: 59406


Ion Ratio Lower Upper

63 100

65 32.4 21.8 40.4

83 14.3 9.7 17.9


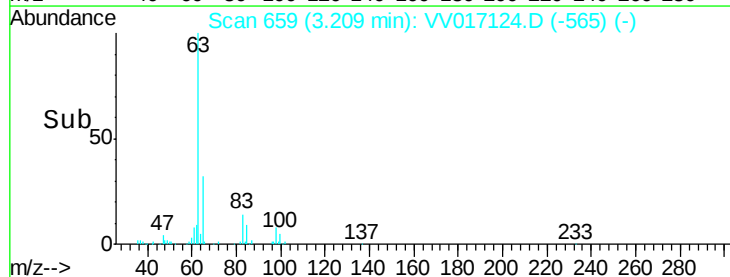
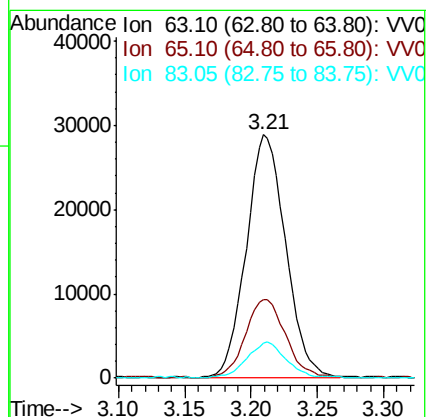
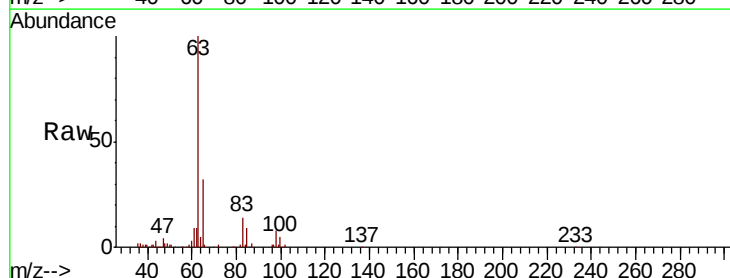


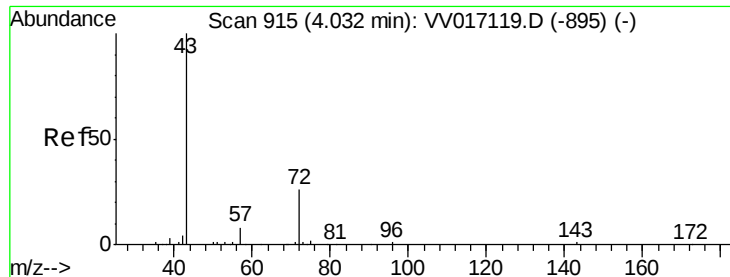

#21
 2-Butanone
 Concen: 29.834 ug/L
 RT: 4.12 min Scan# 943
 Delta R.T. 0.09 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59




Instrument :
 MSVOA_V
 ClientSampled :
 BFXK8DL


Tot Ion: 43 Resp: 76145
 Ion Ratio Lower Upper
 43 100
 72 0.1 12.4 37.4#

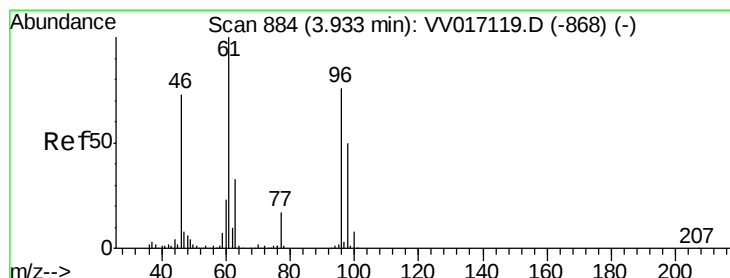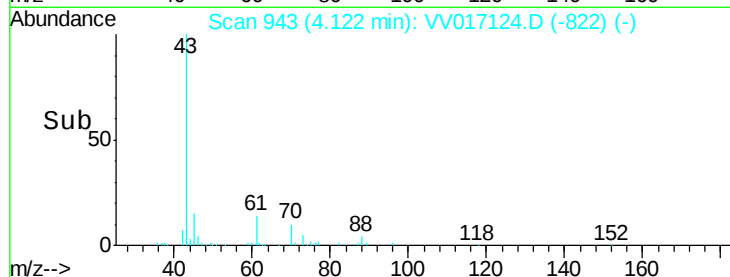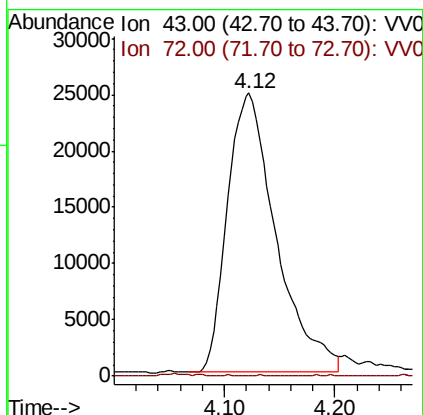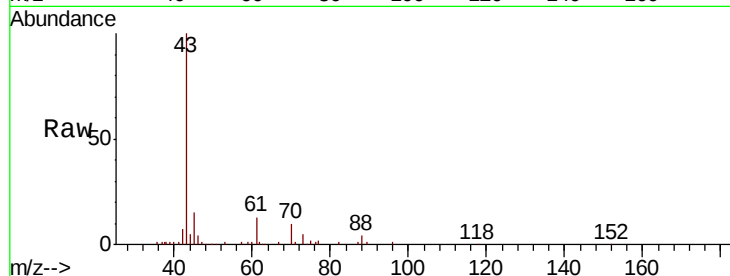

#22
 cis-1,2-Dichloroethene
 Concen: 5.298 ug/L
 RT: 3.94 min Scan# 886
 Delta R.T. 0.01 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59

Tgt Ion: 96 Resp: 64521
 Ion Ratio Lower Upper
 96 100
 61 136.7 91.0 169.0
 68 0.0 0.0 0.0

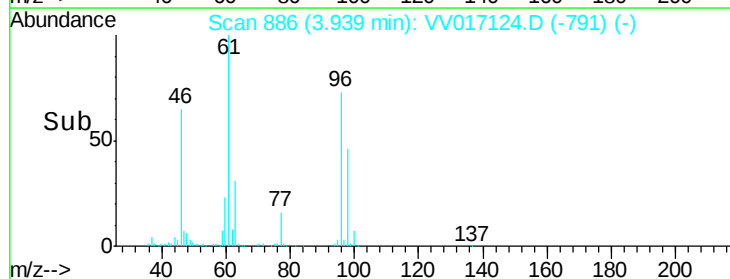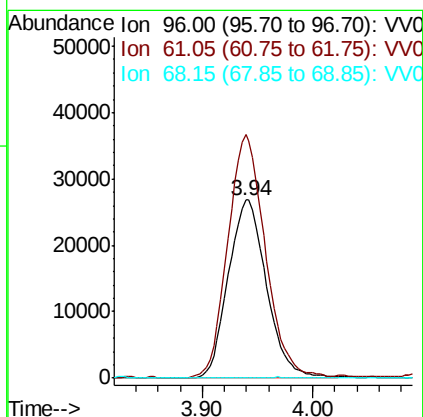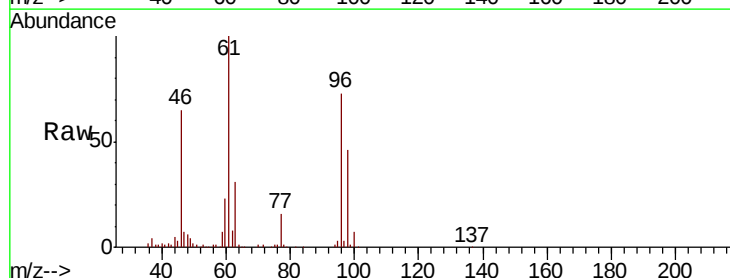

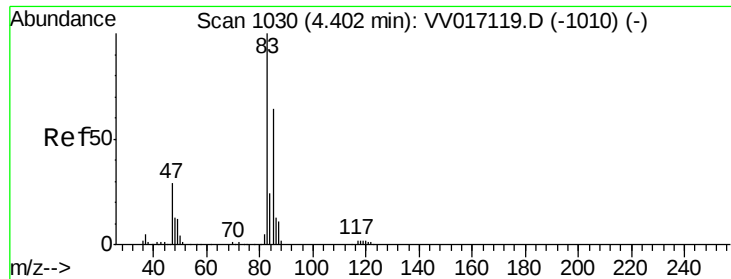

#25

Chloroform

Concen: 0.184 ug/L

RT: 4.40 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :





BFXK8DL

Tot Ion: 83 Resp: 4027

Ion Ratio Lower Upper

83 100

85 76.4 44.2 82.2

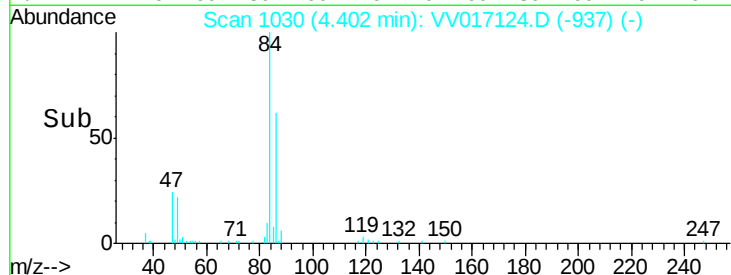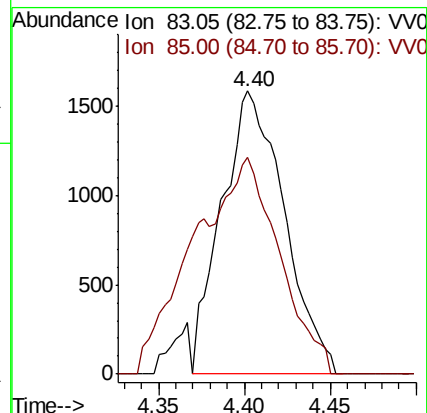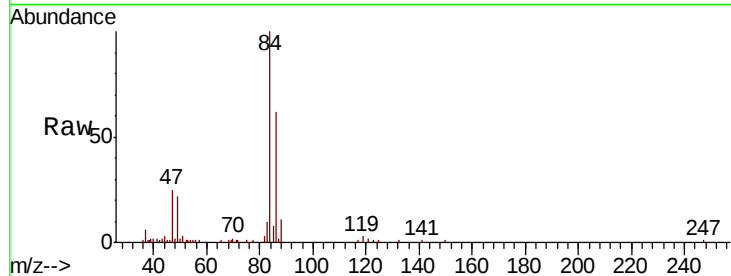

#27

1,2-Dichloroethane

Concen: 0.141 ug/L

RT: 5.16 min Scan# 1266

Delta R.T. 0.00 min

Lab File: VV017124.D




Acq: 25 Jun 2020 13:59


Tgt Ion: 62 Resp: 1914

Ion Ratio Lower Upper

62 100

98 12.6 6.7 10.1#



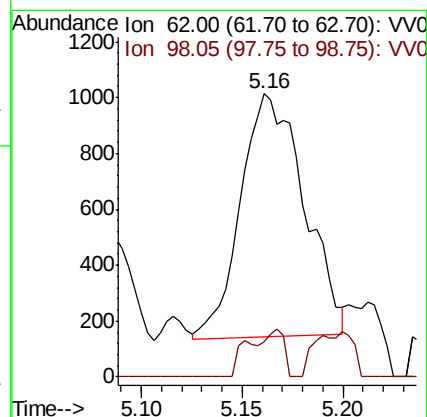



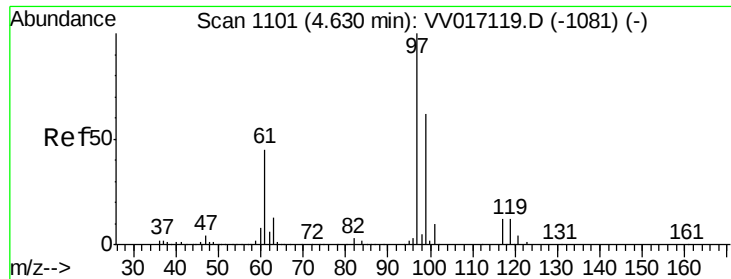

#29
 1,1,1-Trichloroethane
 Concen: 0.815 ug/L
 RT: 4.63 min Scan# 1102
 Delta R.T. 0.00 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59




Instrument :
 MSVOA_V
 ClientSampleId :
 BFXK8DL


Tot Ion: 97 Resp: 16555
 Ion Ratio Lower Upper
 97 100
 99 64.9 50.3 75.5
 61 48.5 36.0 54.0

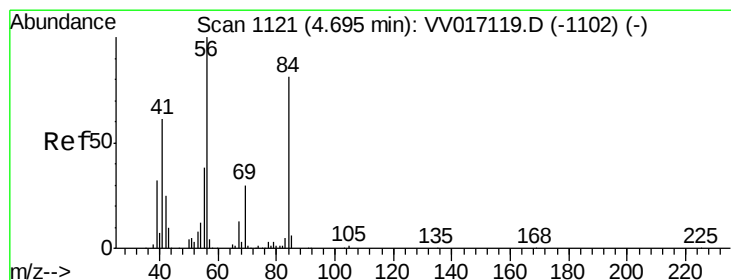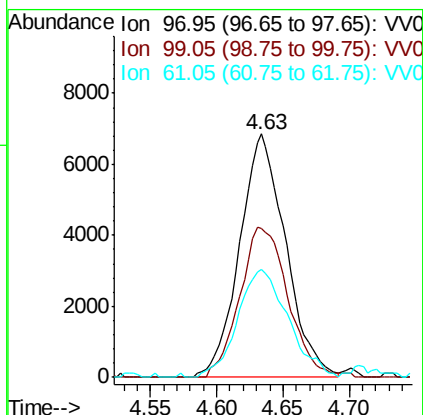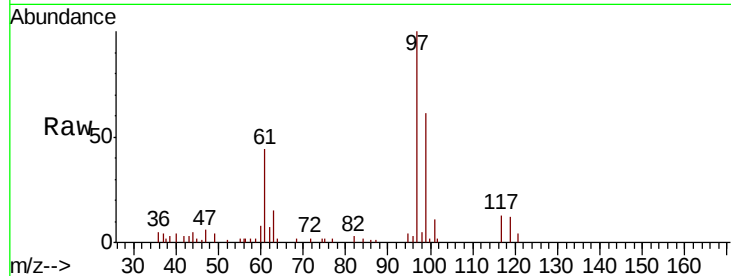

#30
 Cyclohexane
 Concen: 0.395 ug/L
 RT: 4.69 min Scan# 1121
 Delta R.T. -0.00 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59

Tgt Ion: 56 Resp: 7624
 Ion Ratio Lower Upper
 56 100
 69 30.2 24.4 36.6
 84 91.8 69.9 104.9

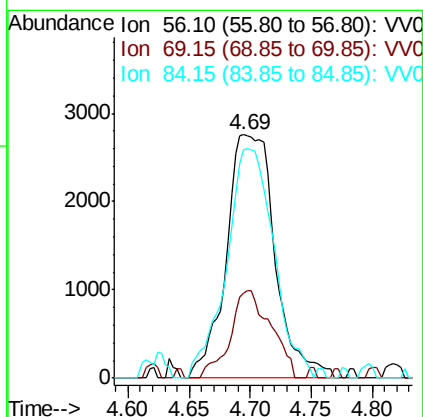



#31

Carbon tetrachloride

Concen: 0.108 ug/L

RT: 4.64 min Scan# 1103

Delta R.T. -0.21 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :


BFXK8DL

Tot Ion:117 Resp: 1982

Ion Ratio Lower Upper




117 100

119 109.9 77.8 116.8

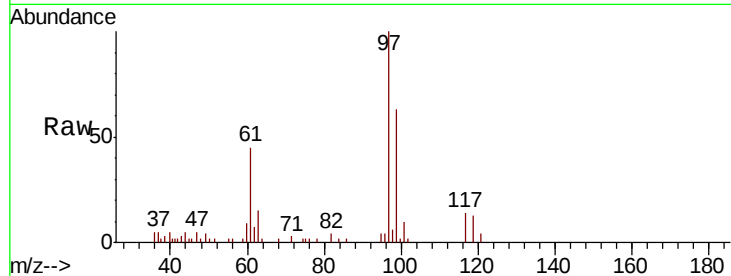

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 118.90 (118.60 to 119.60): V

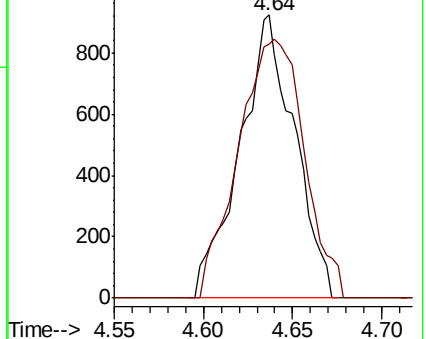

#33

Benzene

Concen: 0.320 ug/L


RT: 5.13 min Scan# 1256

Delta R.T. 0.01 min



Lab File: VV017124.D


Acq: 25 Jun 2020 13:59

Tgt Ion: 78 Resp: 14223



Abundance Ion 78.10 (77.80 to 78.80): VV0

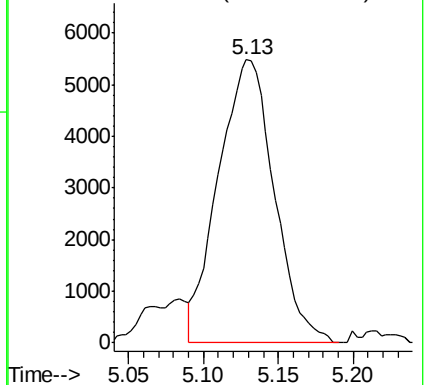

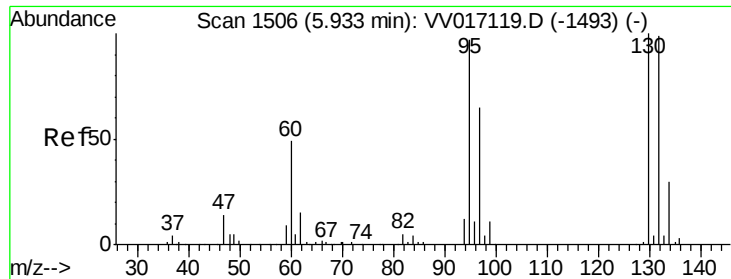

#34

Trichloroethene

Concen: 0.122 ug/L

RT: 5.94 min Scan# 1509

Delta R.T. 0.01 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :

BFXK8DL

Tot Ion: 95 Resp: 1588


Ion Ratio Lower Upper

95 100

97 63.5 45.3 84.1

132 115.8 68.8 127.8

130 112.5 70.2 130.4

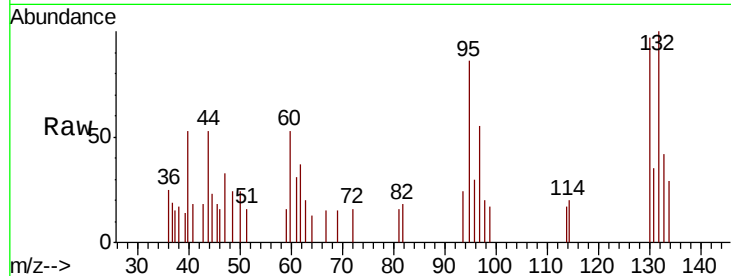




Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): VV0

Ion 129.95 (129.65 to 130.65): VV0

Time-->

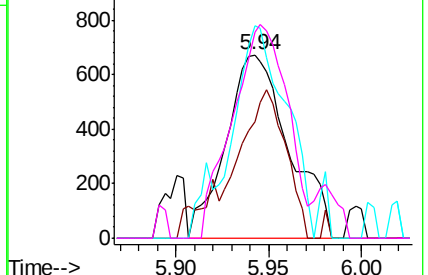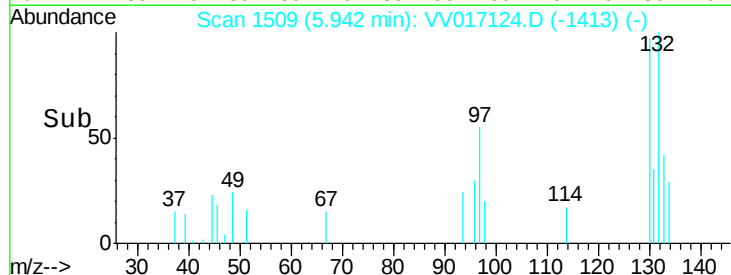

#35

Methylcyclohexane

Concen: 0.841 ug/L

RT: 6.10 min Scan# 1557

Delta R.T. -0.05 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59


Tgt Ion: 83 Resp: 16997

Ion Ratio Lower Upper

83 100

55 1.3 63.6 95.4#

98 0.2 38.8 58.2#






Abundance Ion 83.15 (82.85 to 83.85): VV0

Ion 55.10 (54.80 to 55.80): VV0

Ion 98.15 (97.85 to 98.85): VV0

Time-->

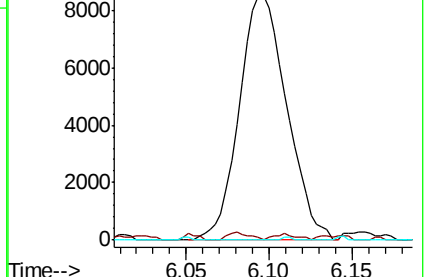

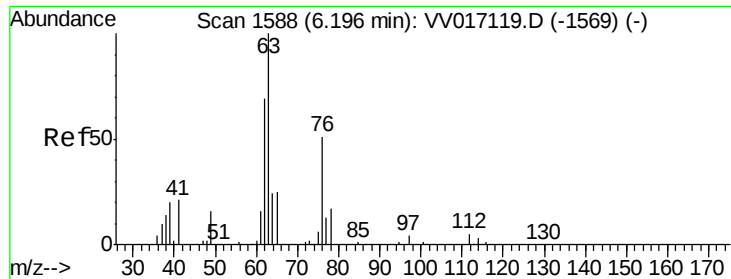

#37

1,2-Dichloropropane

Concen: 0.765 ug/L

RT: 6.10 min Scan# 1557

Delta R.T. -0.10 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :





BFXK8DL

Tot Ion: 63 Resp: 8409

Ion Ratio Lower Upper

63 100

112 0.5 4.4 6.6#

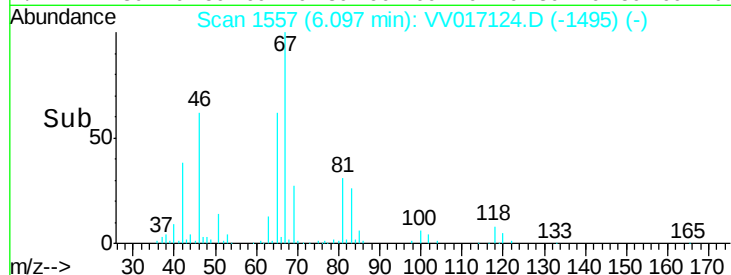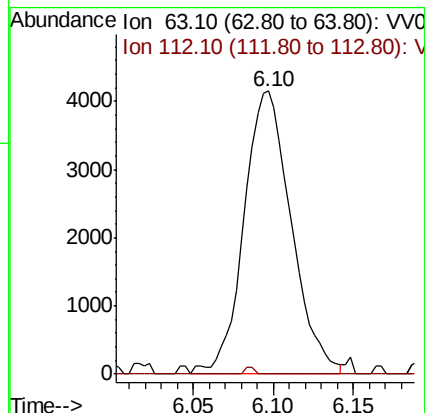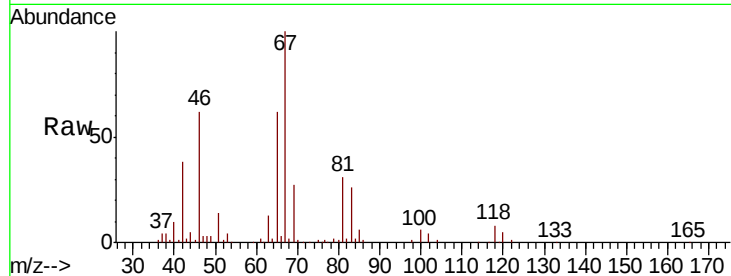

#39

cis-1,3-Dichloropropene

Concen: 0.127 ug/L

RT: 7.01 min Scan# 1841

Delta R.T. -0.04 min

Lab File: VV017124.D




Acq: 25 Jun 2020 13:59


Tgt Ion: 75 Resp: 2076

Ion Ratio Lower Upper

75 100

77 65.5 22.3 41.5#

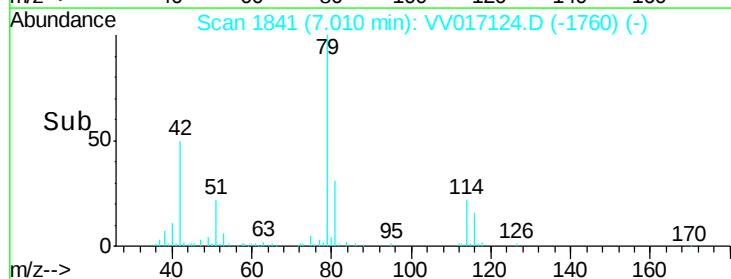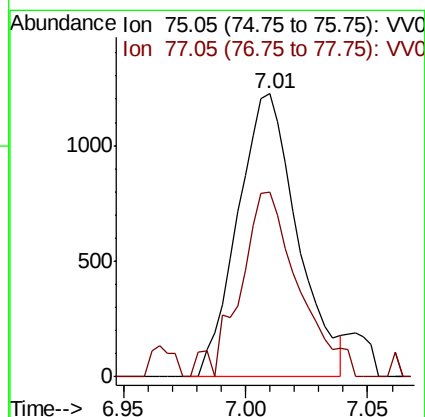



#43

1,3,5-Trimethylbenzene

Concen: 0.123 ug/L

RT: 11.36 min Scan# 3194

Delta R.T. 0.80 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :





BFXK8DL

Tot Ion:105 Resp: 5692

Ion Ratio Lower Upper

105 100

120 39.1 38.6 57.8

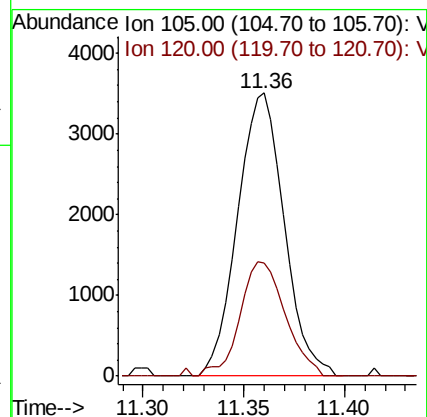

#46

trans-1,3-Dichloropropene

Concen: 0.098 ug/L

RT: 7.64 min Scan# 2038

Delta R.T. -0.03 min

Lab File: VV017124.D




Acq: 25 Jun 2020 13:59


Tgt Ion: 75 Resp: 1378

Ion Ratio Lower Upper

75 100

77 52.0 22.3 41.3#

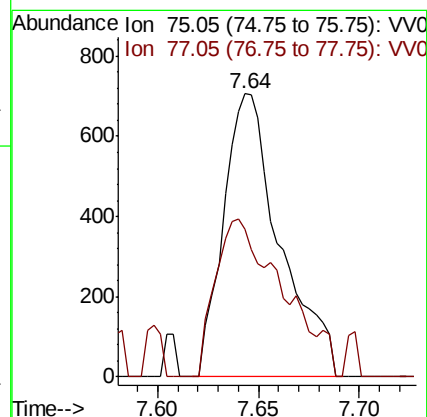


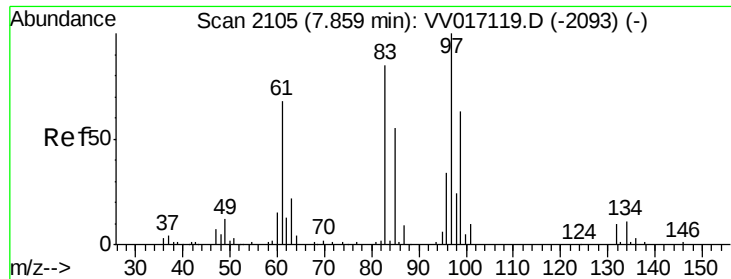




#47
 1,1,2-Trichloroethane
 Concen: 0.325 ug/L
 RT: 7.87 min Scan# 2108
 Delta R.T. 0.01 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXK8DL

Tot Ion:	97	Resp:	2535
Ion	Ratio	Lower	Upper
97	100		
99	46.8	43.6	81.0
83	56.1	57.4	106.6#
85	46.3	38.8	72.0

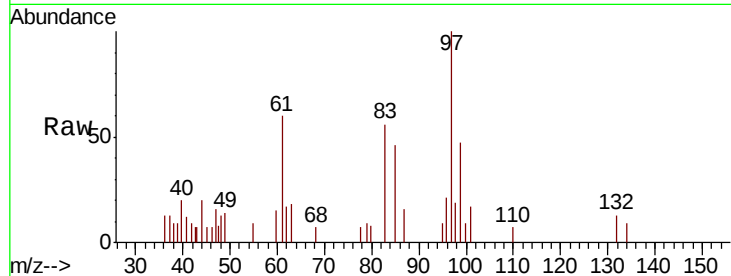


Abundance Ion 96.95 (96.65 to 97.65): VV017124.D (-2093) (-)


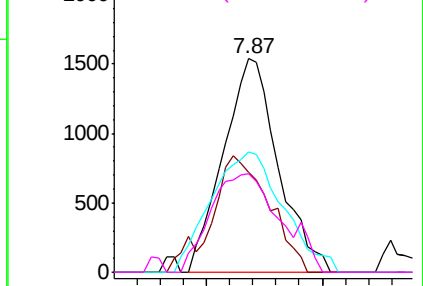



#53
 Chlorobenzene
 Concen: 1.412 ug/L
 RT: 8.90 min Scan# 2430
 Delta R.T. 0.00 min
 Lab File: VV017124.D
 Acq: 25 Jun 2020 13:59

Tgt Ion:	112	Resp:	45420
Ion	Ratio	Lower	Upper
112	100		
114	33.1	22.0	41.0
77	62.0	46.0	69.0



Abundance Ion 112.10 (111.80 to 112.80): VV017124.D (-2415) (-)

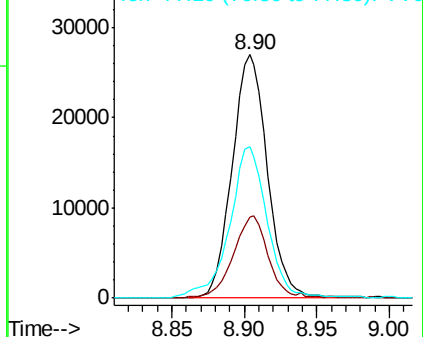


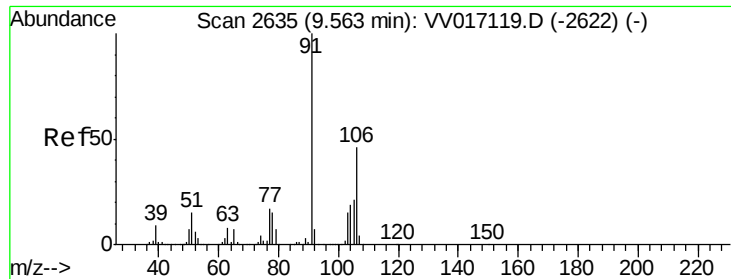




#56
o-xylene
Concen: 0.198 ug/L
RT: 9.56 min Scan# 2635
Delta R.T. -0.00 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59

Instrument :
MSVOA_V
ClientSampleId :
BFXK8DL

Tot Ion:106 Resp: 3998
Ion Ratio Lower Upper
106 100
91 216.4 153.6 285.2

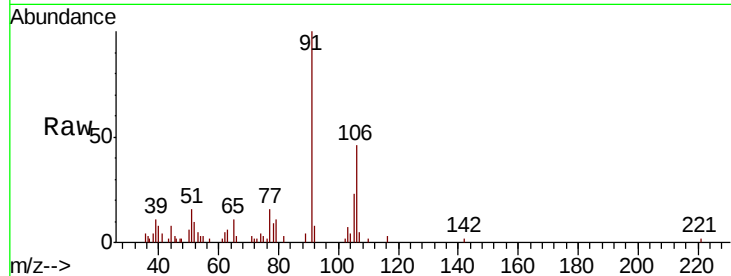


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VV0


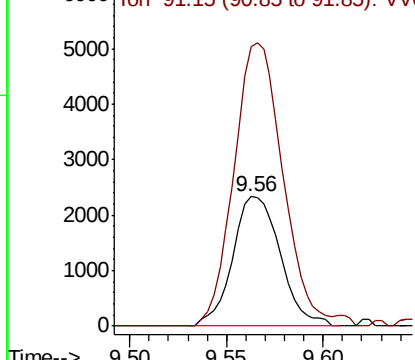



#63
1,3-Dichlorobenzene
Concen: 0.146 ug/L
RT: 11.21 min Scan# 3146
Delta R.T. 0.00 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59

Tgt Ion:146 Resp: 3474
Ion Ratio Lower Upper
146 100
111 27.1 29.2 54.2#
148 57.0 44.9 83.5



Abundance Ion 145.95 (145.65 to 146.65): V
Ion 111.00 (110.70 to 111.70): V
Ion 148.00 (147.70 to 148.70): V




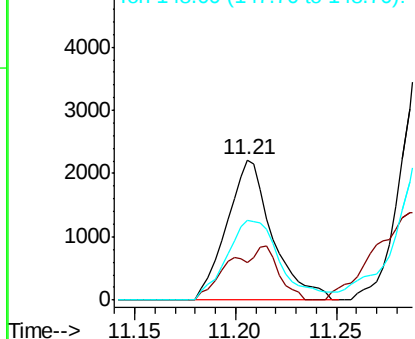


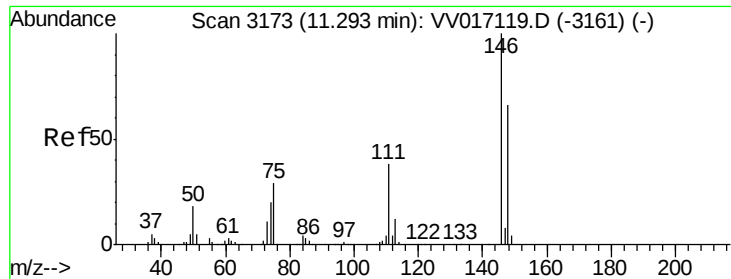

#64
1,4-Dichlorobenzene
Concen: 0.303 ug/L
RT: 11.30 min Scan# 3174
Delta R.T. 0.00 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59




Instrument :
MSVOA_V
ClientSampleId :
BFXK8DL


Tot Ion:146 Resp: 7319
Ion Ratio Lower Upper
146 100
111 34.3 27.4 50.8
148 56.3 44.3 82.3

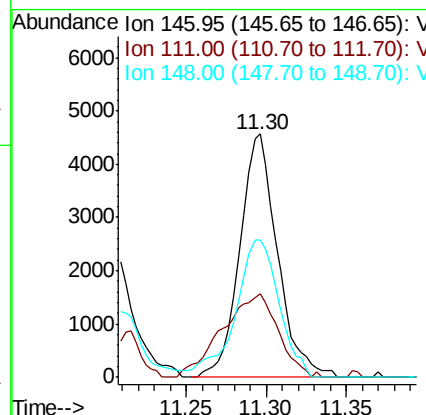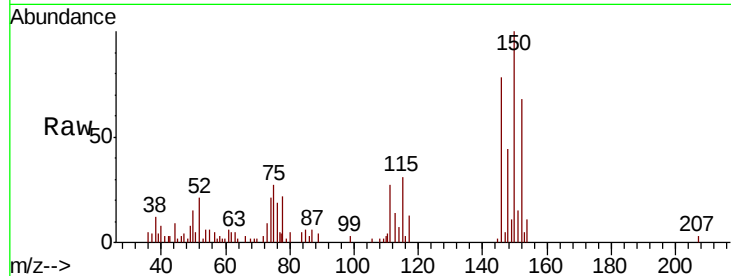

#66
1,2-Dichlorobenzene
Concen: 0.156 ug/L
RT: 11.67 min Scan# 3289
Delta R.T. -0.00 min
Lab File: VV017124.D
Acq: 25 Jun 2020 13:59

Tgt Ion:146 Resp: 3357
Ion Ratio Lower Upper
146 100
111 50.2 34.4 51.6
148 59.4 49.9 74.9

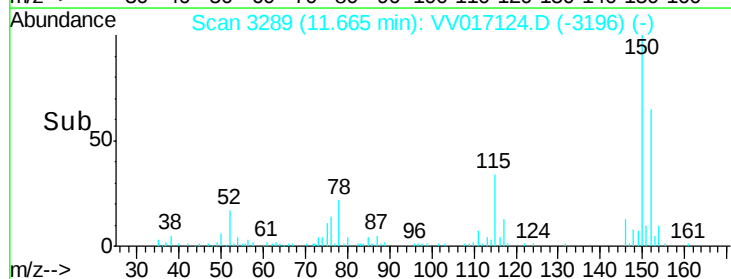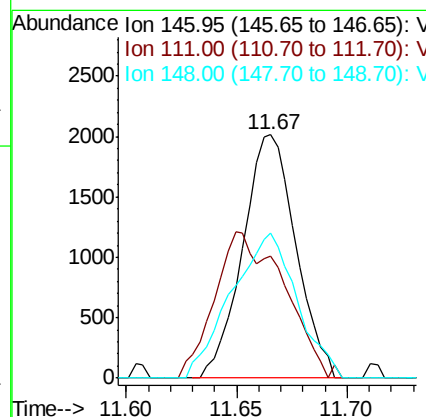



#70

Naphthalene

Concen: 0.132 ug/L

RT: 13.53 min Scan# 3869

Delta R.T. 0.00 min

Lab File: VV017124.D

Acq: 25 Jun 2020 13:59

Instrument :

MSVOA_V

ClientSampleId :

BFXK8DL


Tot Ion:128 Resp: 2935

Ion Ratio Lower Upper

128 100

129 13.0 8.8 13.2

127 5.6 10.5 15.7#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

