


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VW062520\
Data File : VW017137.D
Acq On : 25 Jun 2020 19:11
Operator : SY/MD
Sample : L3106-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXM9

Manual Integrations
APPROVED

MMDadoda
6/26/2020 2:07:35 PM

Quant Time: Jun 26 03:50:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 01:31:34 2020
Response via : Initial Calibration

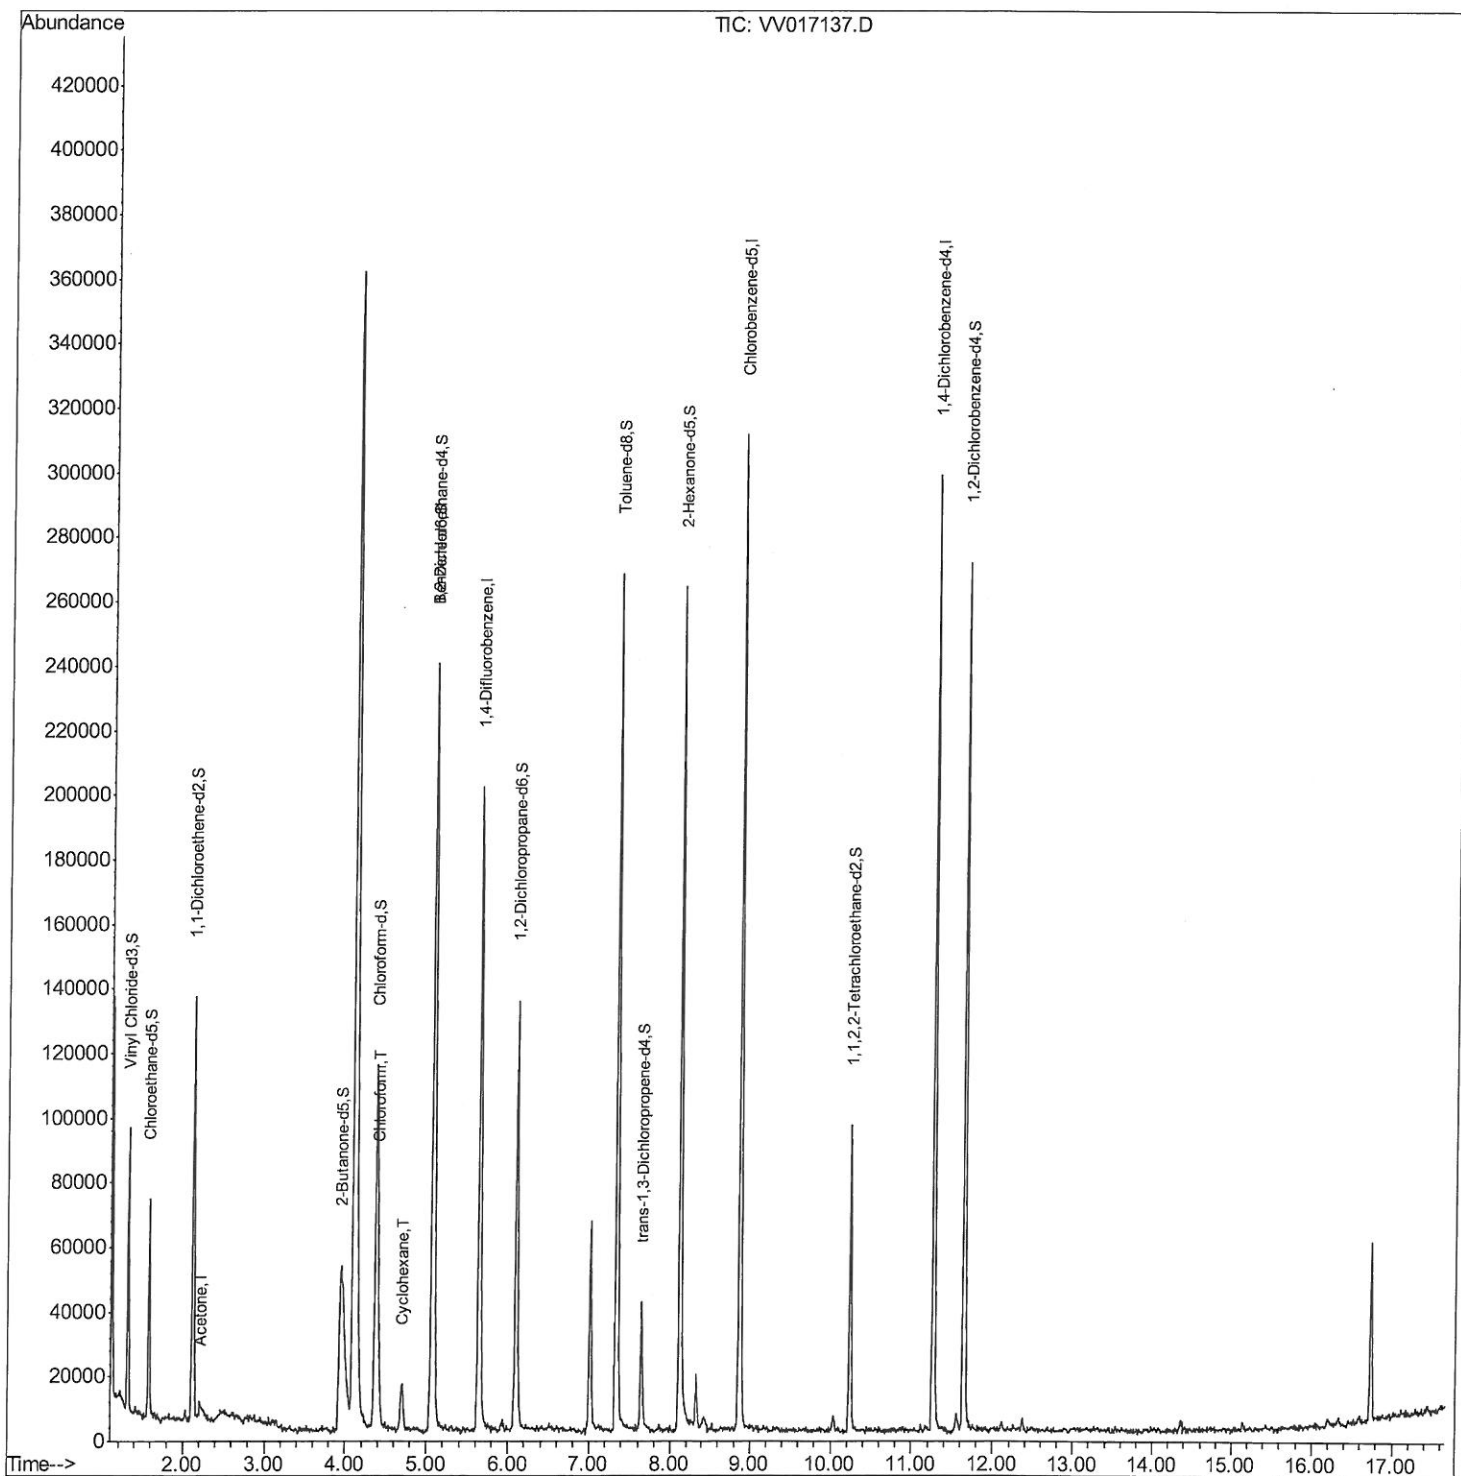

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
Data File : VV017137.D
Acq On : 25 Jun 2020 19:11
Operator : SY/MD
Sample : L3106-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXM9

Manual Integrations
APPROVED

MMDadoda
6/26/2020 2:07:35 PM

Quant Time: Jun 26 01:37:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 01:31:34 2020
Response via : Initial Calibration

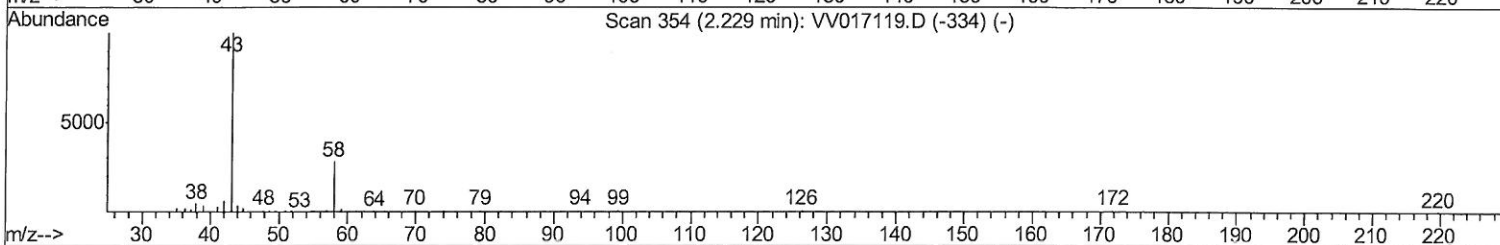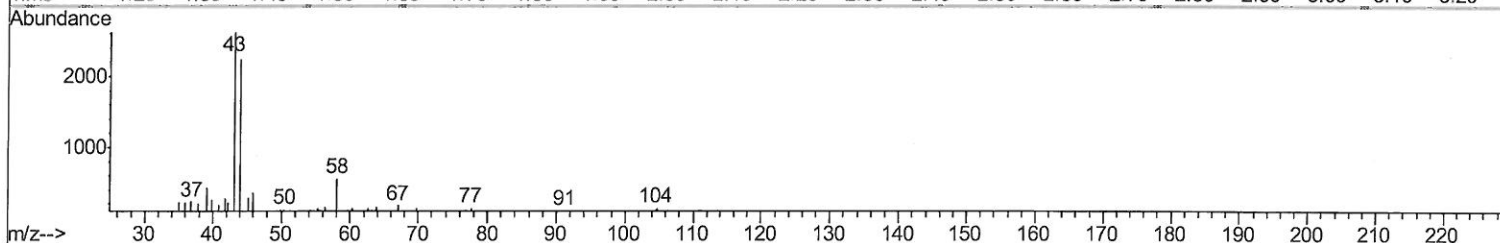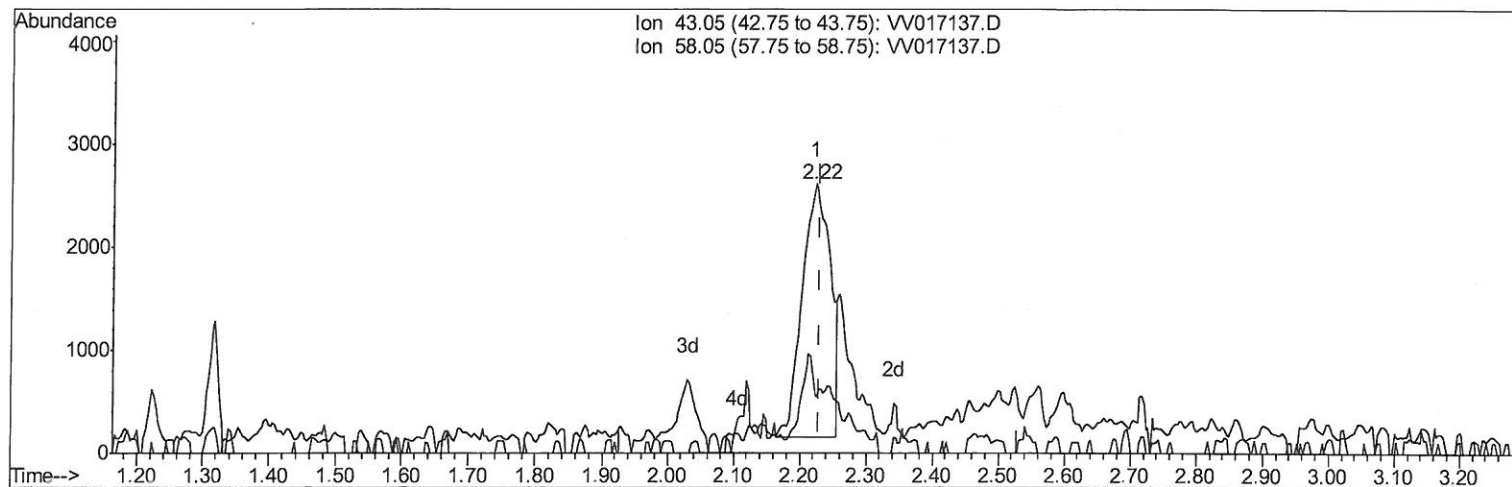

TIC: VV017137.D

(13) Acetone (T)

2.222min (-0.007) 5.72ug/L

response 7235

Ion	Exp%	Act%
43.05	100	100
58.05	29.20	0.62
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017137.D
 Acq On : 25 Jun 2020 19:11
 Operator : SY/MD
 Sample : L3106-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXM9

Manual Integrations
 APPROVED

MMDadoda
 6/26/2020 2:07:35 PM

Quant Time: Jun 26 01:37:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 01:31:34 2020
 Response via : Initial Calibration

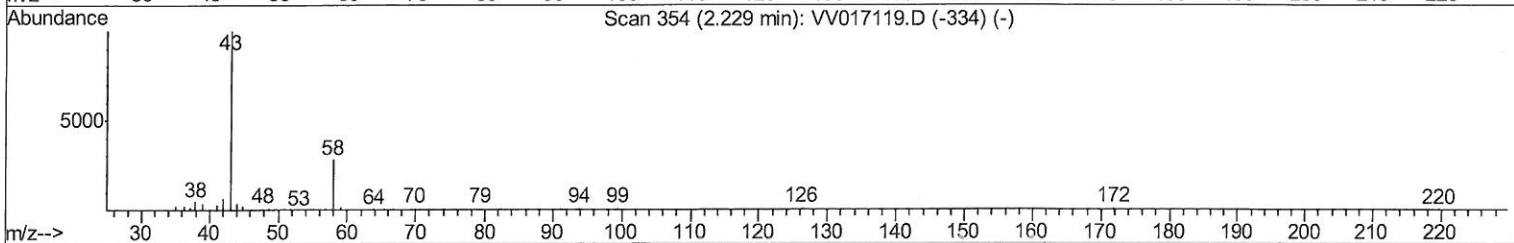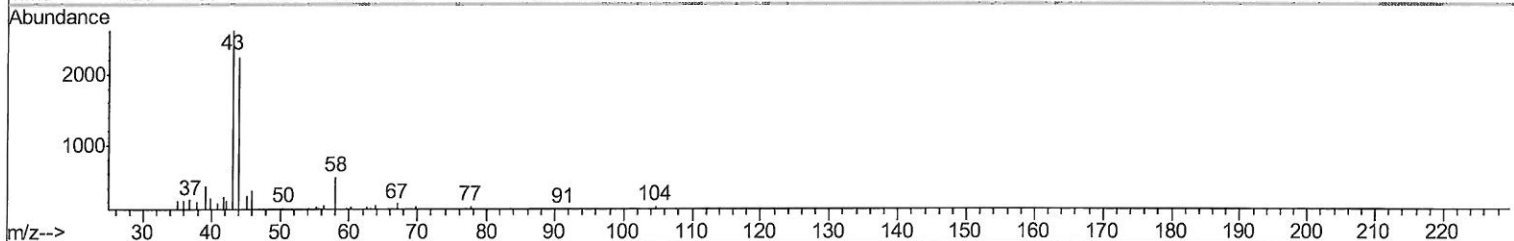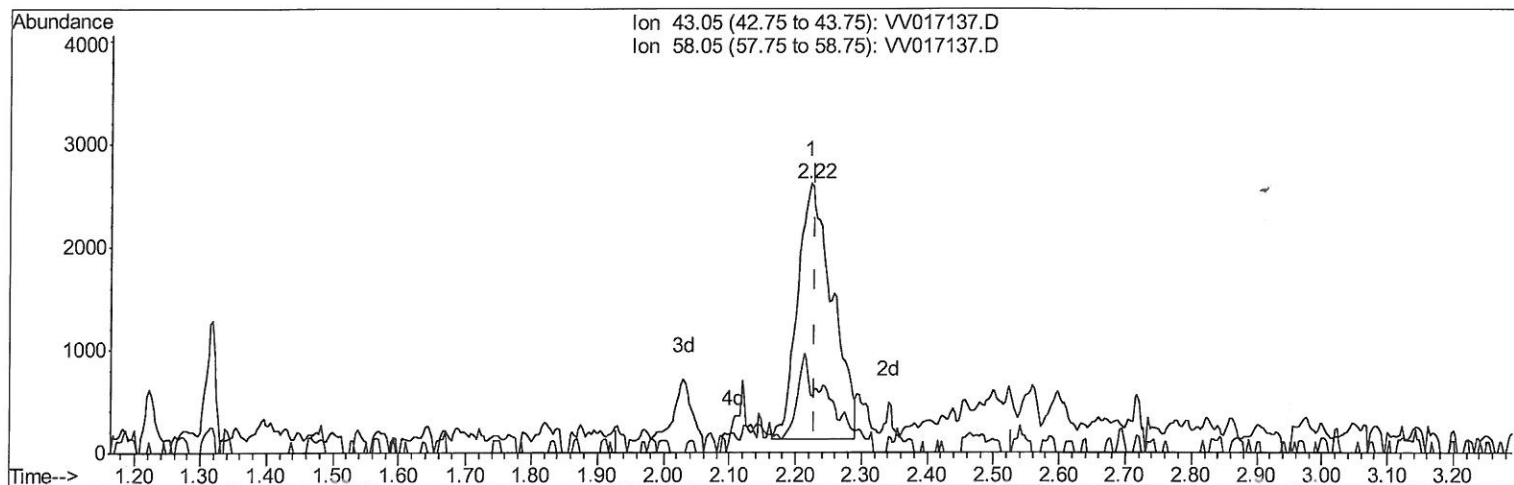

TIC: VV017137.D

(13) Acetone (T)

2.222min (-0.007) 7.25ug/L m

response 9168

Ion	Exp%	Act%
43.05	100	100
58.05	29.20	0.49
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 06/29/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017137.D
 Acq On : 25 Jun 2020 19:11
 Operator : SY/MD
 Sample : L3106-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 BFXM9

Manual Integrations
 APPROVED

MMDadoda
 6/26/2020 2:07:35 PM

Quant Time: Jun 26 03:50:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 01:31:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	163620	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	161474	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	73555	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	49800	5.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.40%
7) Chloroethane-d5	1.58	69	38223	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.12	63	72092	3.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.20%
20) 2-Butanone-d5	3.95	46	116502	46.55	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.10%
24) Chloroform-d	4.38	84	106980	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.06	65	57495	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.07	84	195331	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.10	67	57049	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	7.34	98	170385	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
45) trans-1,3-Dichloropropene-	7.64	79	21677	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
48) 2-Hexanone-d5	8.11	63	83824	42.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.24%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	39418	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	67171	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%

Target Compounds

					Ovalue	
13) Acetone	2.22	43	9168m	7.246	ug/L	
25) Chloroform	4.41	83	12860	0.630	ug/L	87
30) Cyclohexane	4.70	56	7424	0.403	ug/L	97

> MB
 6/29/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed