

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017162.D
 Acq On : 26 Jun 2020 06:00
 Operator : SY/MD
 Sample : L3068-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9F45

Quant Time: Jun 26 07:03:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 05:12:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	168648	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	167831	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	78179	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46580	4.60	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.00%
7) Chloroethane-d5	1.58	69	38243	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.00%
11) 1,1-Dichloroethene-d2	2.13	63	67206	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.93	46	110185	42.71	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.42%
24) Chloroform-d	4.38	84	98952	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.06	65	52837	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
32) Benzene-d6	5.08	84	184471	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.80%
36) 1,2-Dichloropropane-d6	6.10	67	53543	4.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.20%
41) Toluene-d8	7.34	98	156498	3.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.60%
45) trans-1,3-Dichloropropene-	7.64	79	20073	3.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.00%
48) 2-Hexanone-d5	8.11	63	76262	36.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.74%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	37418	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	64718	4.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.60%


Target Compounds					Ovalue
13) Acetone	2.22	43	8139	6.241 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062520\
Data File : VV017162.D
Acq On : 26 Jun 2020 06:00
Operator : SY/MD
Sample : L3068-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9F45

Quant Time: Jun 26 07:03:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 05:12:03 2020
Response via : Initial Calibration

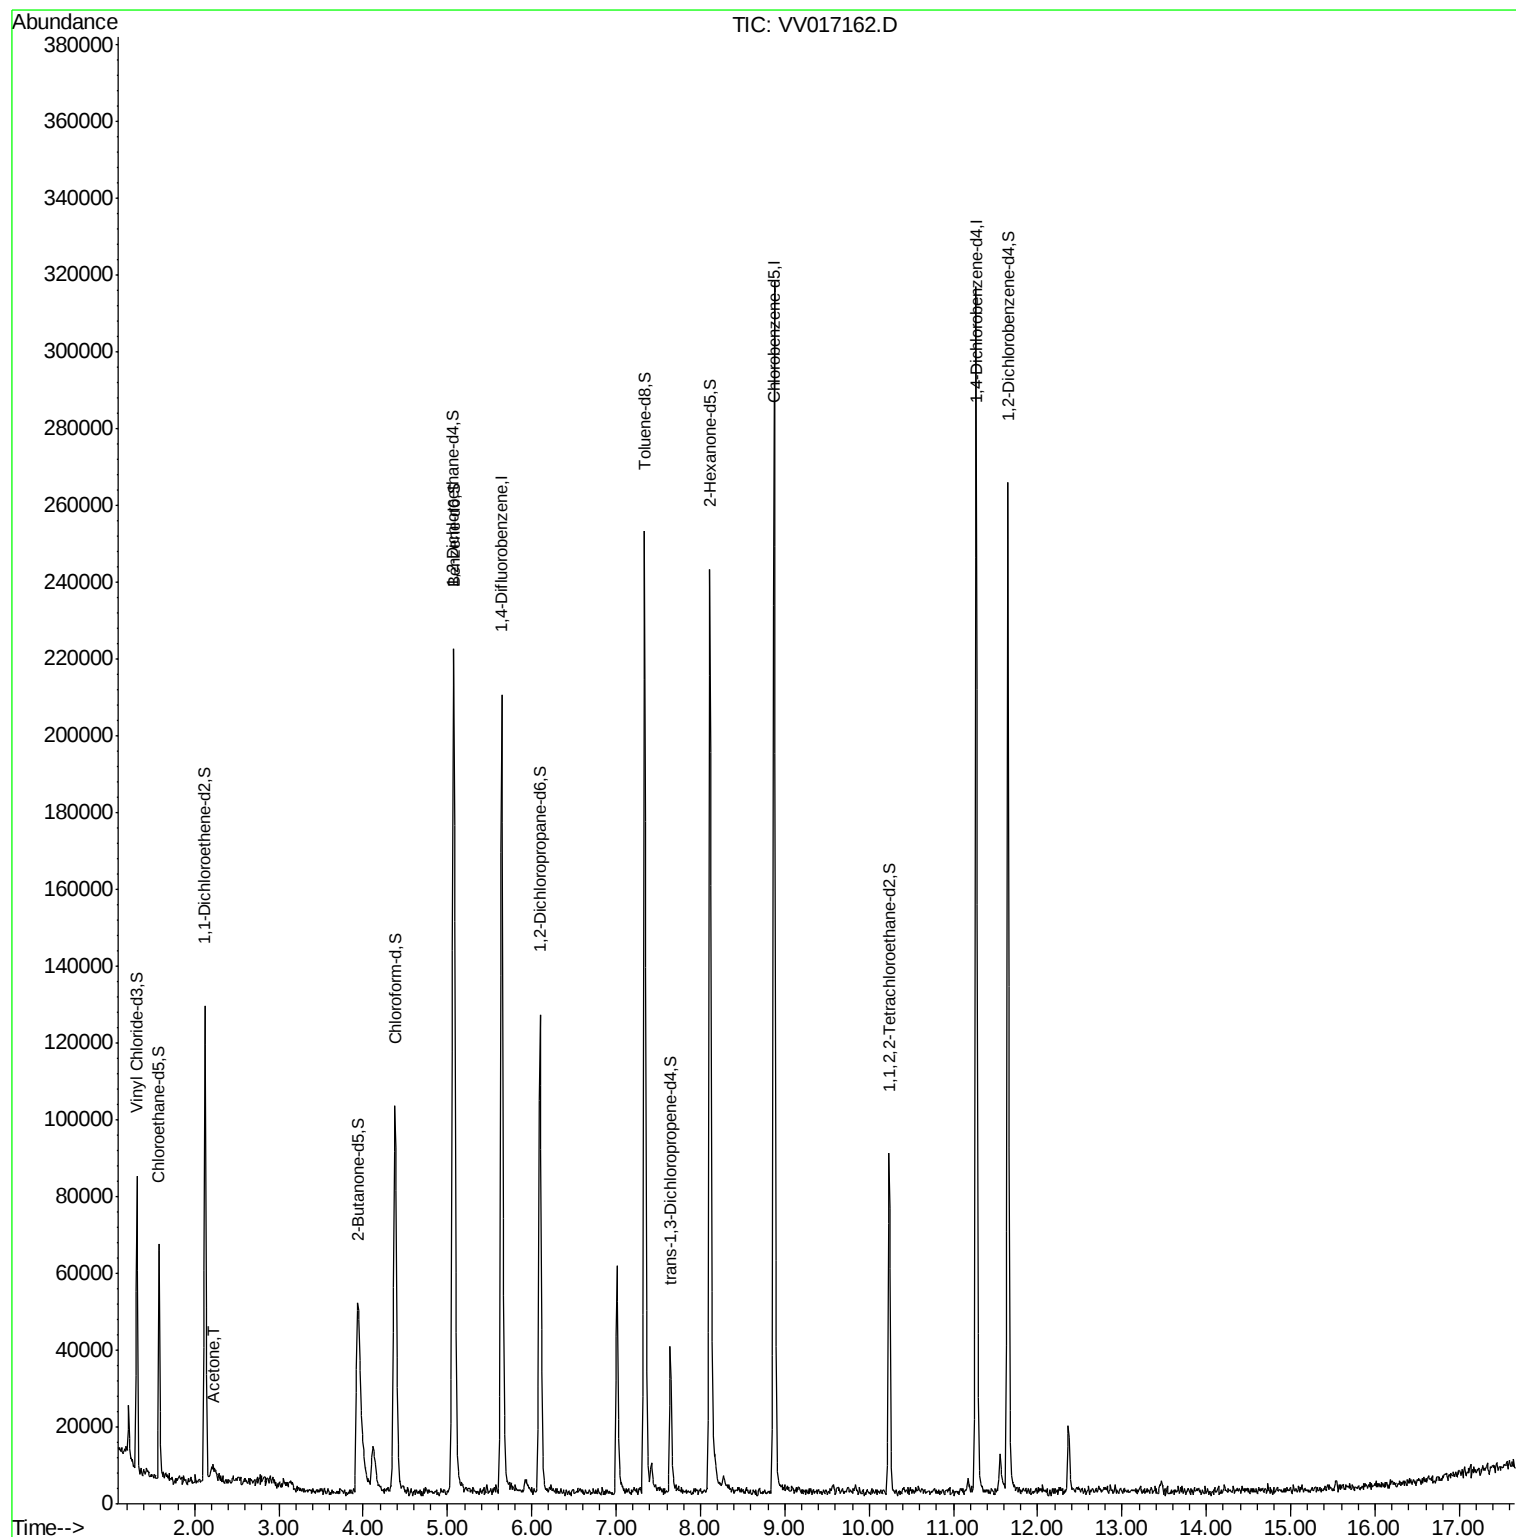

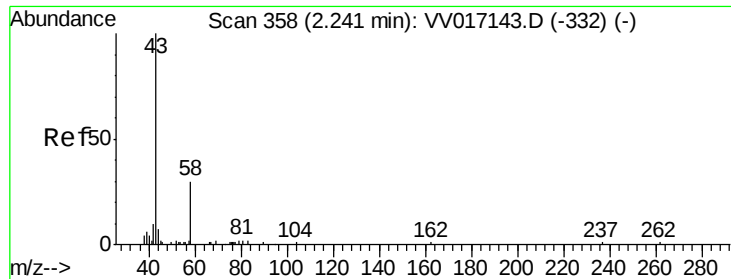

#13

Acetone

Concen: 6.241 ug/L

RT: 2.22 min Scan# 352

Delta R.T. -0.02 min

Lab File: VV017162.D

Acq: 26 Jun 2020 06:00

Instrument :

MSVOA_V

ClientSampleId :

F9F45

Tot Ion: 43 Resp: 8139

Ion Ratio Lower Upper

43 100

58 21.3 0.0 58.4

