

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017163.D
 Acq On : 26 Jun 2020 06:24
 Operator : SY/MD
 Sample : L3107-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXP2

Quant Time: Jun 26 07:06:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 05:12:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	164817	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	163608	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	75067	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48660	4.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.40%
7) Chloroethane-d5	1.58	69	38456	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.13	63	68059	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.93	46	114879	45.57	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.14%
24) Chloroform-d	4.38	84	101848	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.06	65	54077	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.08	84	185668	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
36) 1,2-Dichloropropane-d6	6.10	67	54235	4.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.40%
41) Toluene-d8	7.34	98	159431	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.00%
45) trans-1,3-Dichloropropene-	7.64	79	19788	3.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.80%
48) 2-Hexanone-d5	8.11	63	78315	38.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.68%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	37868	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	66245	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	8120	6.371 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062520\
Data File : VV017163.D
Acq On : 26 Jun 2020 06:24
Operator : SY/MD
Sample : L3107-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXP2

Quant Time: Jun 26 07:06:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 05:12:03 2020
Response via : Initial Calibration

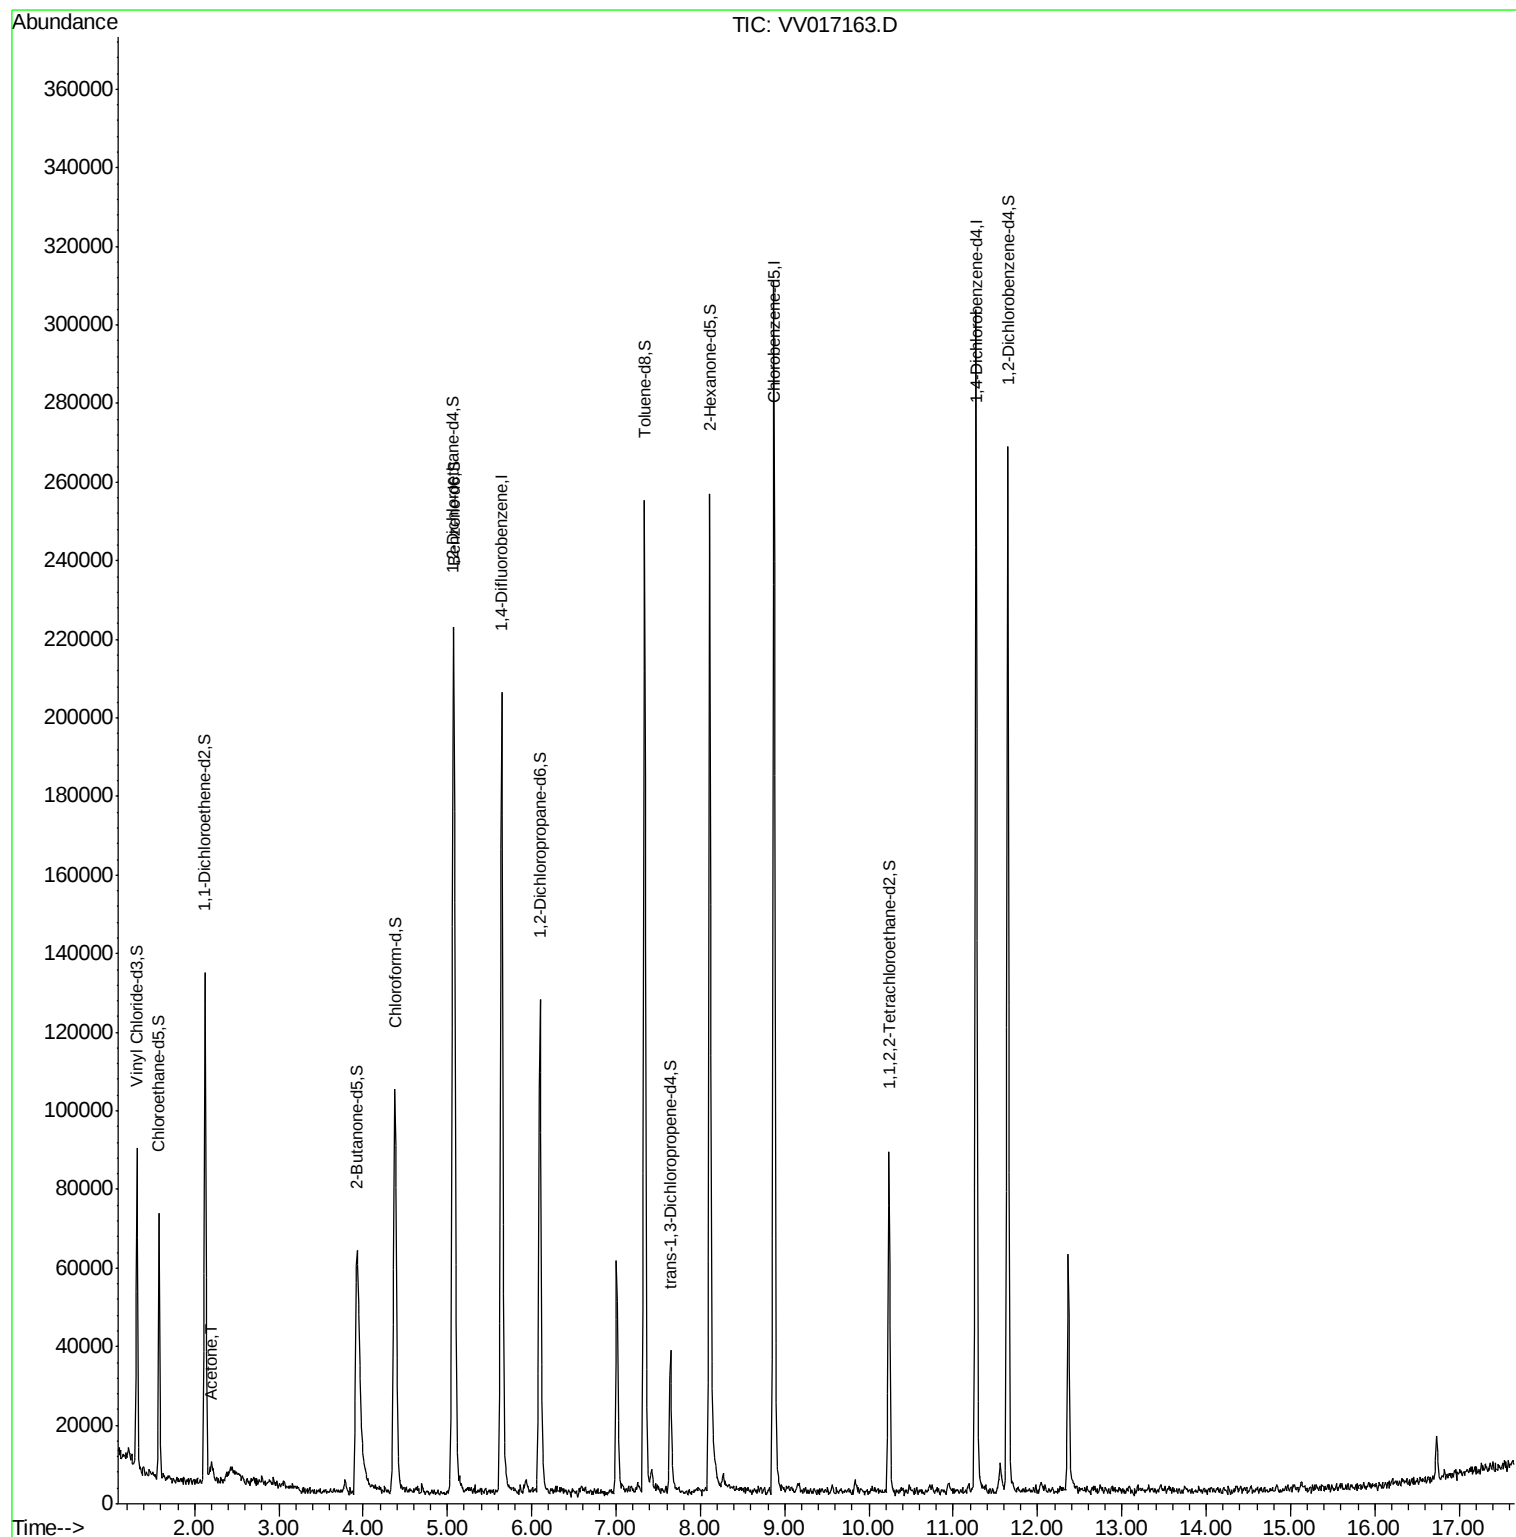

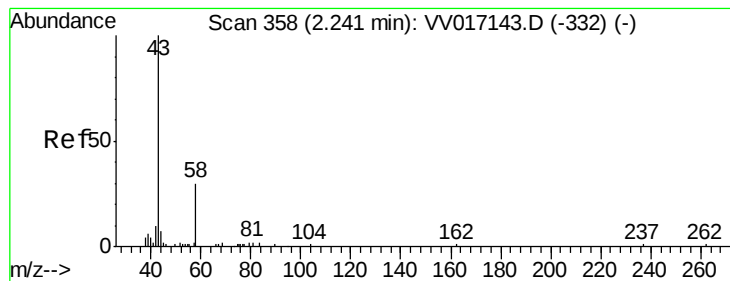

#13
 Acetone
 Concen: 6.371 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.04 min
 Lab File: VV017163.D
 Acq: 26 Jun 2020 06:24

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXP2

Tot Ion: 43 Resp: 8120
 Ion Ratio Lower Upper
 43 100
 58 21.4 0.0 58.4

