

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062520\
 Data File : VV017173.D
 Acq On : 26 Jun 2020 11:10
 Operator : SY/MD
 Sample : L3107-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXP2

Quant Time: Jun 26 13:24:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 12:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	164150	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	163570	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	76719	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45552	4.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.40%
7) Chloroethane-d5	1.58	69	38248	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%
11) 1,1-Dichloroethene-d2	2.12	63	68447	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	3.92	46	115668	46.07	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.14%
24) Chloroform-d	4.38	84	102112	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.06	65	55277	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.08	84	184300	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
36) 1,2-Dichloropropane-d6	6.09	67	53633	4.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.40%
41) Toluene-d8	7.34	98	159997	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.40%
45) trans-1,3-Dichloropropene-	7.64	79	20550	3.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.60%
48) 2-Hexanone-d5	8.11	63	78734	39.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.10%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	37679	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	65457	4.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	7355	5.795 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062520\
Data File : VV017173.D
Acq On : 26 Jun 2020 11:10
Operator : SY/MD
Sample : L3107-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXP2

Quant Time: Jun 26 13:24:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 12:57:45 2020
Response via : Initial Calibration

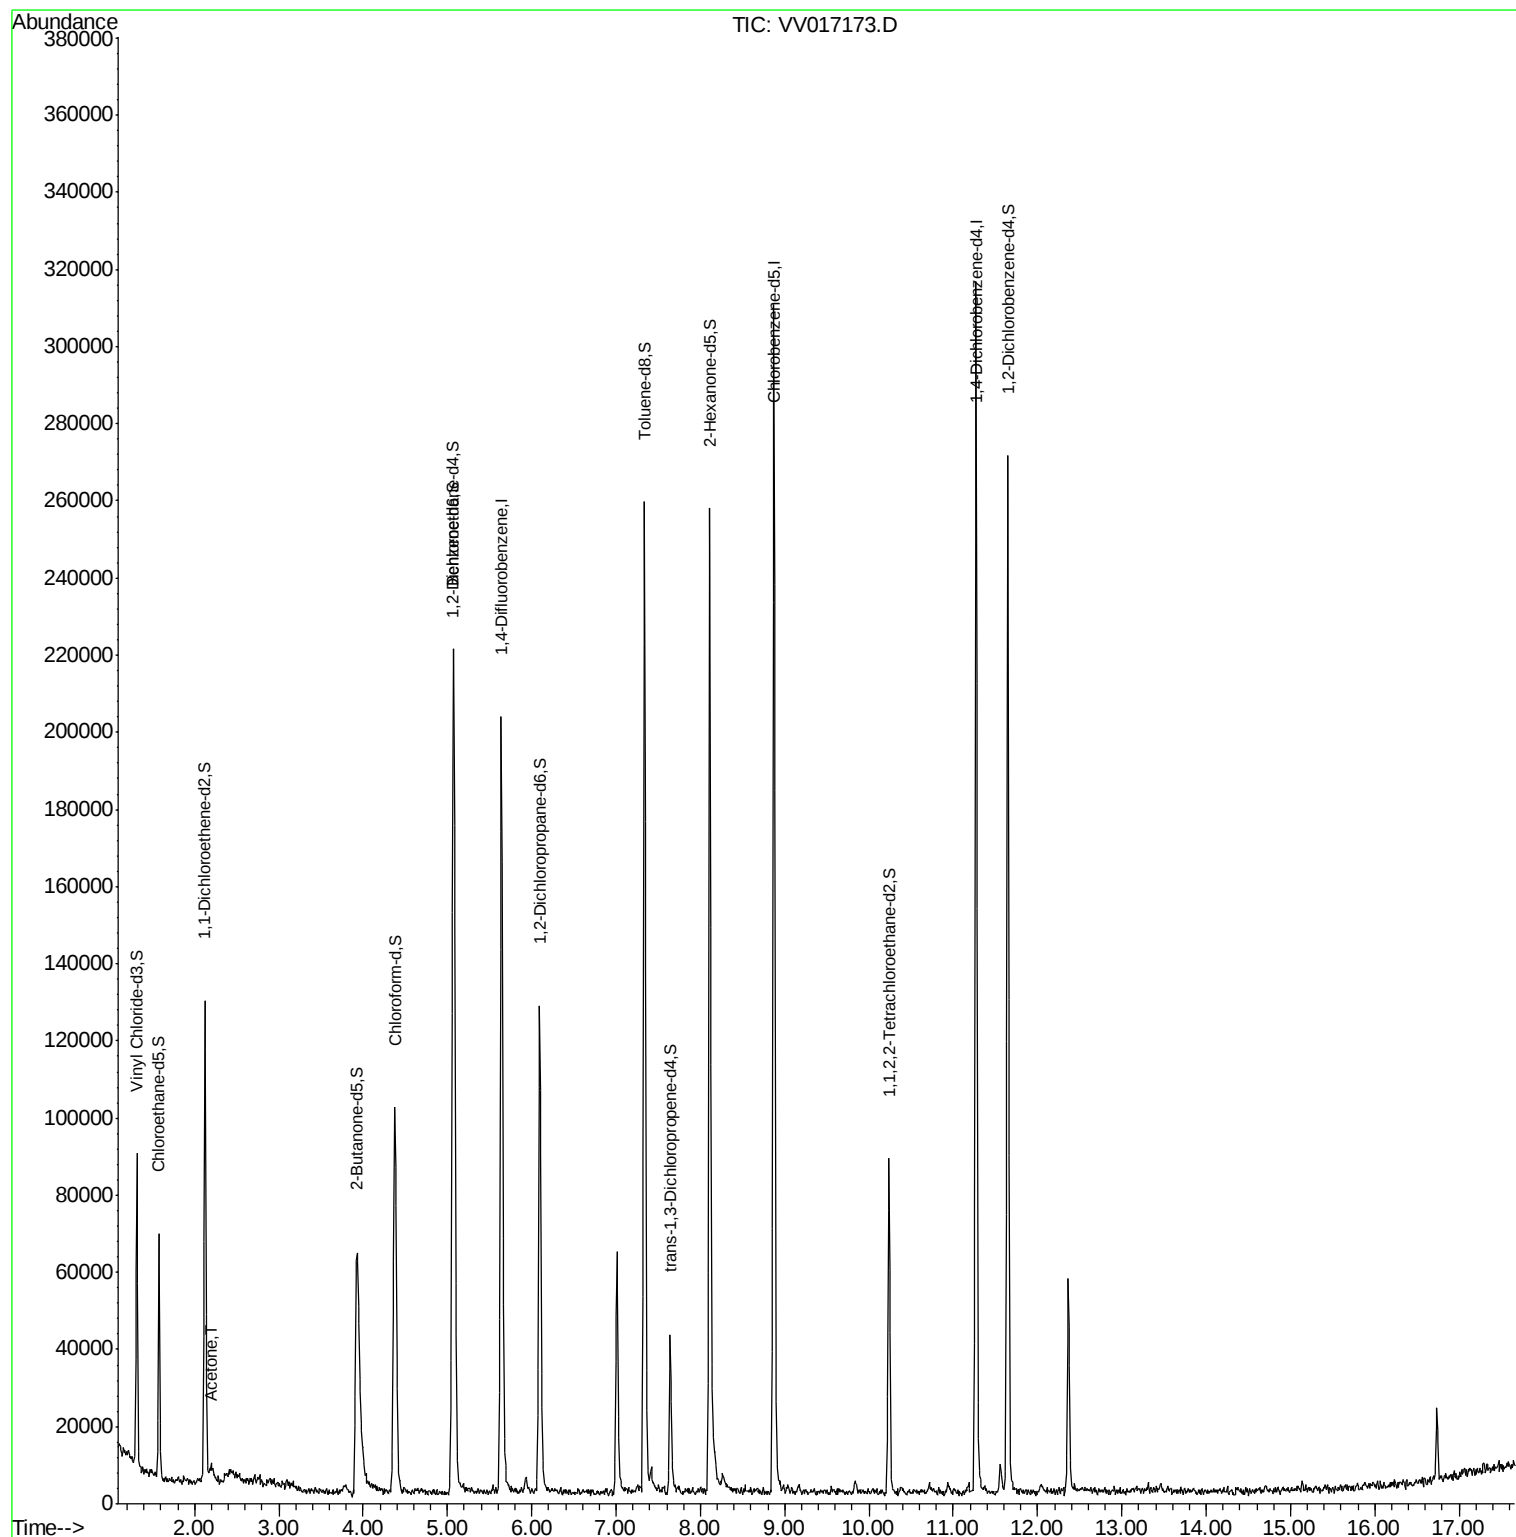

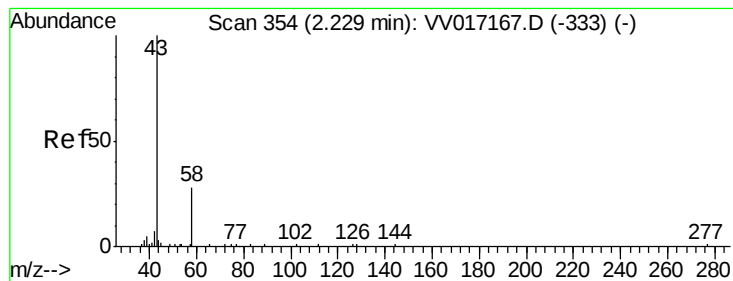

#13

Acetone

Concen: 5.795 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.05 min

Lab File: VV017173.D

Acq: 26 Jun 2020 11:10

Instrument :
MSVOA_V
ClientSampleId :
BFXP2

Tot Ion: 43 Resp: 7355

Ion Ratio Lower Upper

43 100

58 35.6 0.0 58.4

