

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062618\
 Data File : VV006466.D
 Acq On : 26 Jun 2018 14:47
 Operator : SY/MD
 Sample : J3673-08
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DAZA3

Quant Time: Jun 27 02:34:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 27 02:22:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	296671	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	266595	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	119058	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	83249	4.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.40%
7) Chloroethane-d5	1.58	69	66398	4.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.60%
11) 1,1-Dichloroethene-d2	2.13	63	113426	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	3.95	46	179510	49.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.22%
24) Chloroform-d	4.41	84	147671	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	5.09	65	74418	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.11	84	327586	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.12	67	98330	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.37	98	292492	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.67	79	27789	3.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.00%
46) 2-Hexanone-d5	8.14	63	135454	44.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	55274	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	106540	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	10389	4.64	ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062618\
Data File : VV006466.D
Acq On : 26 Jun 2018 14:47
Operator : SY/MD
Sample : J3673-08
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DAZA3

Quant Time: Jun 27 02:34:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 27 02:22:39 2018
Response via : Initial Calibration

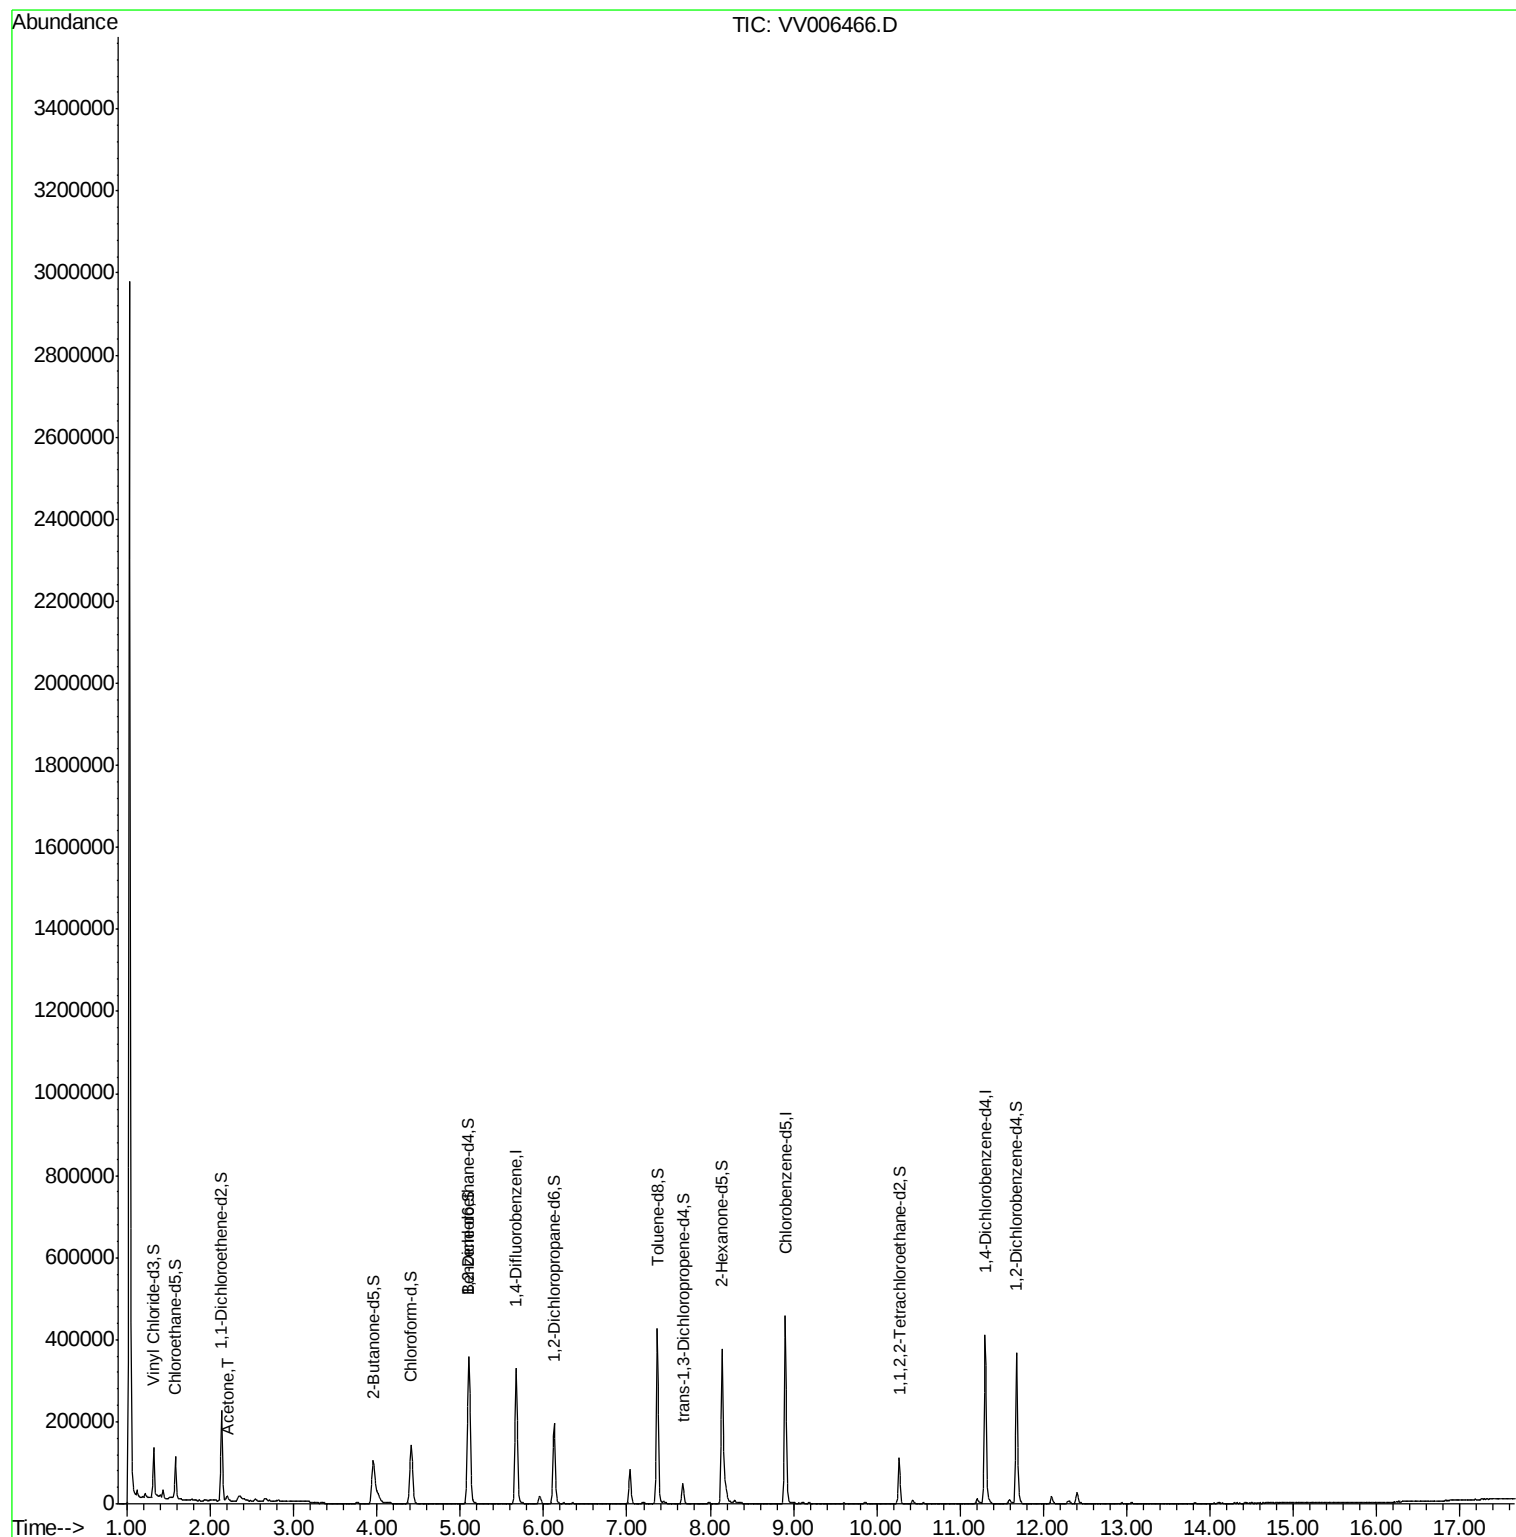

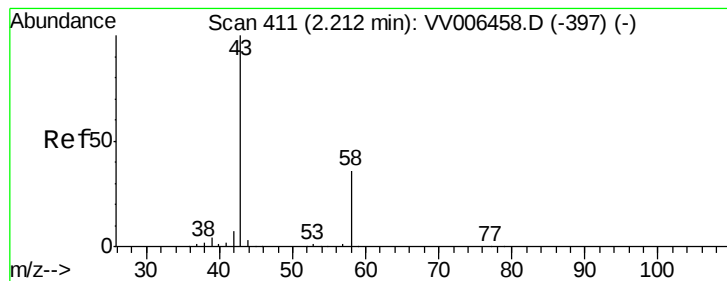

#13

Acetone

Concen: 4.64 ug/L

RT: 2.20 min Scan# 408

Delta R.T. -0.01 min

Lab File: VV006466.D

Acq: 26 Jun 2018 14:47


Instrument :
MSVOA_V
ClientSampleId :
DAZA3

Tot Ion: 43 Resp: 10389

Ion Ratio Lower Upper

43 100

58 37.9 0.0 77.4

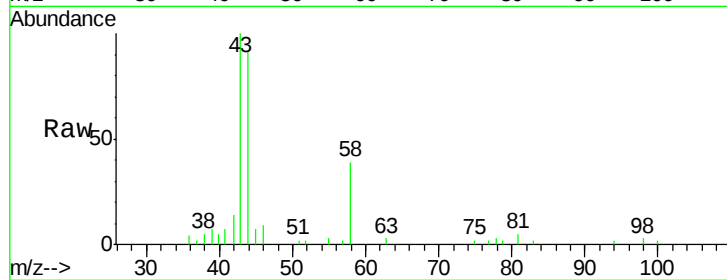

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

