


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062618\
 Data File : VV006457.D
 Acq On : 26 Jun 2018 09:23
 Operator : SY/MD
 Sample : BFB80
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 28 01:18:56 2018

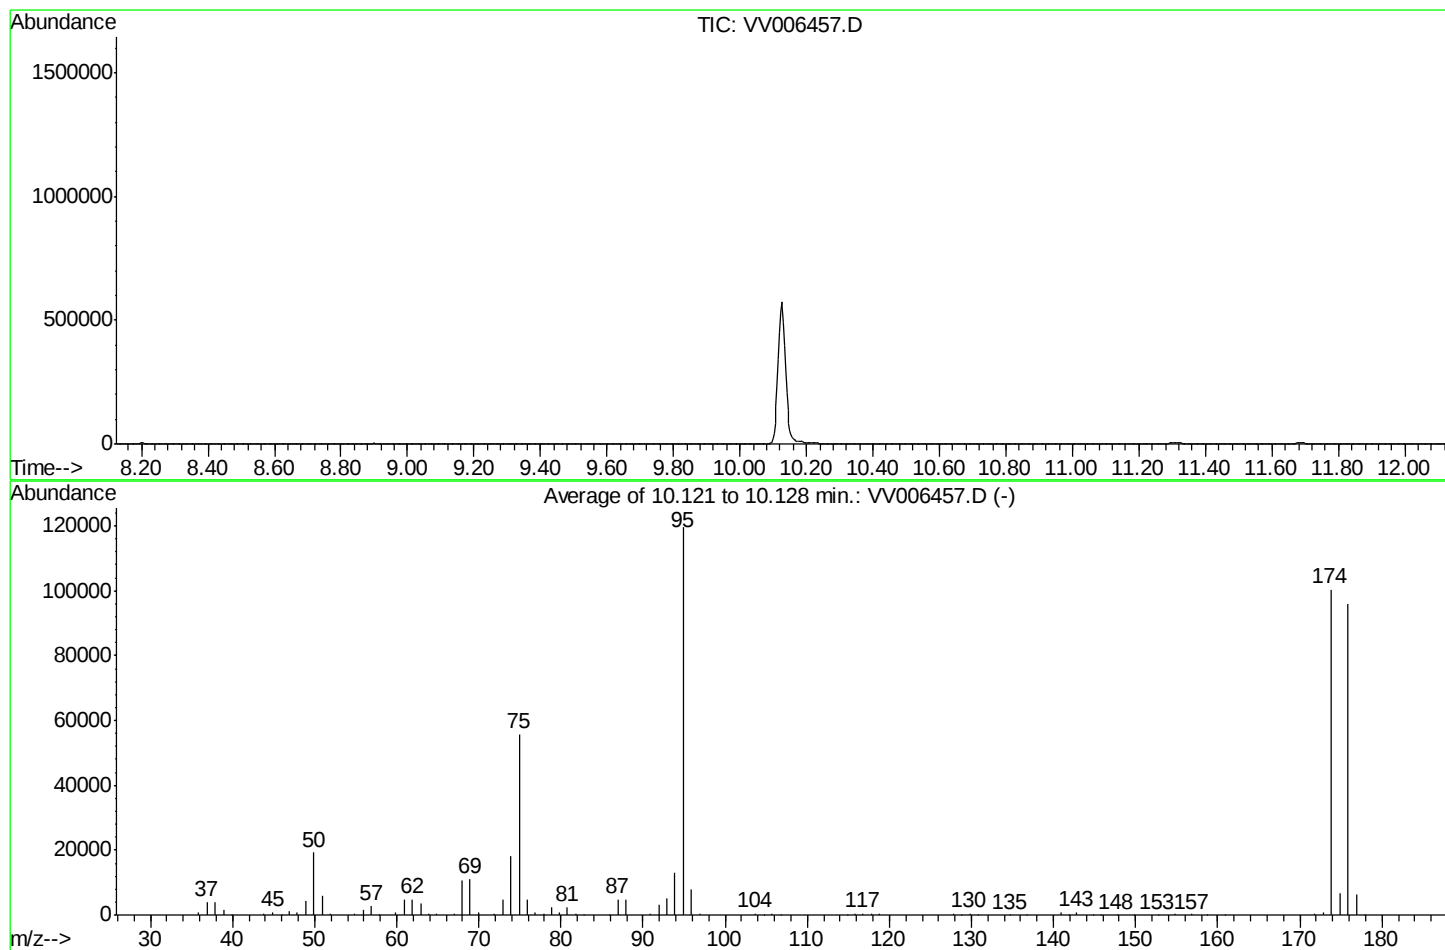

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	19189	PASS
75	95	30	80	46.6	55768	PASS
95	95	100	100	100.0	119565	PASS
96	95	5	9	6.5	7771	PASS
173	174	0.00	2	0.7	732	PASS
174	95	50	120	83.9	100322	PASS
175	174	5	9	6.8	6823	PASS
176	174	95	101	95.7	96002	PASS
177	176	5	9	6.5	6232	PASS

Scan 2858 (10.080 min): VV006457.D
BFB80

m/z	Abundance
39.70	170.0
43.90	629.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
35.90	728.0
36.90	3915.0
37.90	3709.0
39.00	1479.0
39.90	192.0
43.80	1107.0
44.90	762.0
46.00	130.0
46.90	1115.0
47.90	668.0
48.90	4233.0
49.90	19080.0
50.90	6001.0
51.90	287.0
54.80	258.0
55.90	1570.0
56.90	2759.0
57.80	107.0
59.90	990.0
60.90	4726.0
61.90	4720.0
62.90	3712.0
63.90	426.0
64.90	407.0
67.00	234.0
67.90	10381.0
68.90	10851.0
69.90	789.0
71.90	581.0
72.90	4760.0
73.90	17592.0
74.90	53848.0
76.00	4641.0
76.80	785.0
77.80	609.0
78.80	2550.0
79.80	765.0
80.80	2549.0
81.80	552.0
82.80	109.0
85.90	151.0
86.90	4752.0
87.90	4515.0
90.80	358.0
91.90	2953.0
92.90	4776.0
93.90	12702.0
94.90	115976.0
95.90	7560.0
96.90	285.0
103.70	438.0
104.80	140.0
105.70	399.0
106.80	123.0
114.70	104.0
115.80	327.0
116.80	576.0
117.80	363.0
118.80	534.0
127.80	412.0
128.80	196.0
129.80	343.0
130.80	167.0
134.80	153.0
136.80	136.0
140.90	906.0
141.80	124.0
142.80	867.0
144.80	149.0
145.70	139.0
147.70	216.0
149.70	125.0
152.70	105.0
154.80	240.0
156.80	218.0
171.70	451.0
172.90	704.0
173.80	94136.0
174.80	6485.0
175.80	90272.0
176.90	5980.0
177.80	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
35.90	720.0
36.90	4286.0
37.90	4029.0
39.00	1572.0
39.90	232.0
43.80	1073.0
44.90	831.0
46.00	116.0
46.90	1273.0
47.80	691.0
48.90	4385.0
49.90	19880.0
50.90	6133.0
51.90	261.0
54.80	300.0
55.90	1675.0
56.90	2848.0
57.80	115.0
59.90	1001.0
60.90	4950.0
61.90	5082.0
62.90	3862.0
63.90	448.0
64.90	412.0
66.90	267.0
67.90	10923.0
68.90	11457.0
69.90	815.0
71.90	588.0
72.90	4974.0
73.90	18968.0
74.90	57584.0
76.00	4815.0
76.80	816.0
77.80	585.0
78.80	2610.0
79.80	888.0
80.80	2578.0
81.80	556.0
82.80	113.0
86.00	146.0
86.90	5050.0
87.90	4971.0
90.90	346.0
91.90	3099.0
92.90	5148.0
93.90	13336.0
94.90	123624.0
95.90	7972.0
96.90	272.0
103.70	447.0
104.80	154.0
105.80	444.0
106.80	154.0
114.80	108.0
115.80	319.0
116.80	640.0
117.80	345.0
118.80	524.0
127.80	409.0
128.80	216.0
129.80	431.0
130.80	182.0
134.70	170.0
136.80	152.0
140.80	890.0
141.80	129.0
142.80	942.0
144.80	150.0
145.70	169.0
147.70	215.0
149.70	144.0
152.70	132.0
154.70	226.0
156.80	249.0
158.70	110.0
160.80	119.0
171.70	482.0
172.90	750.0
173.80	103992.0
174.90	7012.0
175.80	99424.0
176.90	6472.0
177.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
35.90	662.0
36.90	4149.0
37.90	3853.0
38.90	1490.0
39.90	276.0
43.80	1035.0
44.90	792.0
46.90	1331.0
47.80	658.0
48.90	3988.0
49.90	18608.0
50.90	5784.0
52.00	214.0
54.80	308.0
55.90	1563.0
56.90	2720.0
57.80	113.0
59.90	917.0
60.90	4921.0
61.90	4842.0
62.90	3627.0
63.90	417.0
64.80	408.0
66.90	261.0
67.90	10225.0
68.90	10911.0
69.90	872.0
71.90	568.0
72.90	4745.0
73.90	18088.0
74.90	55872.0
75.90	4560.0
76.80	798.0
77.90	515.0
78.80	2429.0
79.80	834.0
80.80	2449.0
81.80	515.0
86.00	132.0
86.90	4962.0
87.80	4866.0
90.90	296.0
91.90	2939.0
92.90	5022.0
93.90	12751.0
94.90	119096.0
95.90	7783.0
96.90	244.0
103.70	419.0
104.80	143.0
105.80	450.0
106.70	136.0
114.90	108.0
115.80	328.0
116.80	600.0
117.80	300.0
118.80	494.0
127.80	364.0
128.80	218.0
129.80	487.0
130.80	144.0
134.70	177.0
136.70	150.0
140.80	812.0
141.80	124.0
142.80	972.0
144.80	113.0
145.80	172.0
147.70	188.0
149.80	125.0
152.70	115.0
154.70	204.0
156.90	238.0
158.70	108.0
160.90	122.0
171.80	534.0
172.90	743.0
173.80	102840.0
174.90	6972.0
175.80	98312.0
176.90	6244.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80