

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062619\
 Data File : VV011755.D
 Acq On : 26 Jun 2019 11:46
 Operator : SY/MD
 Sample : K3462-11DL 4X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCP7DL

Quant Time: Jun 26 12:21:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 26 12:11:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	182076	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	168451	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	70525	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60281	4.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.80%
7) Chloroethane-d5	1.57	69	40844	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.20%
11) 1,1-Dichloroethene-d2	2.12	63	91355	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	3.95	46	168541	52.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.88%
24) Chloroform-d	4.40	84	117775	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.08	65	67081	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.09	84	242713	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
36) 1,2-Dichloropropane-d6	6.12	67	75232	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.36	98	209298	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.66	79	24124	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.13	63	128895	54.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	50518	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	67890	5.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.00%


Target Compounds					Ovalue
5) Vinyl chloride	1.32	62	92035	5.466 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062619\
Data File : VV011755.D
Acq On : 26 Jun 2019 11:46
Operator : SY/MD
Sample : K3462-11DL 4X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCP7DL

Quant Time: Jun 26 12:21:00 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 26 12:11:41 2019
Response via : Initial Calibration

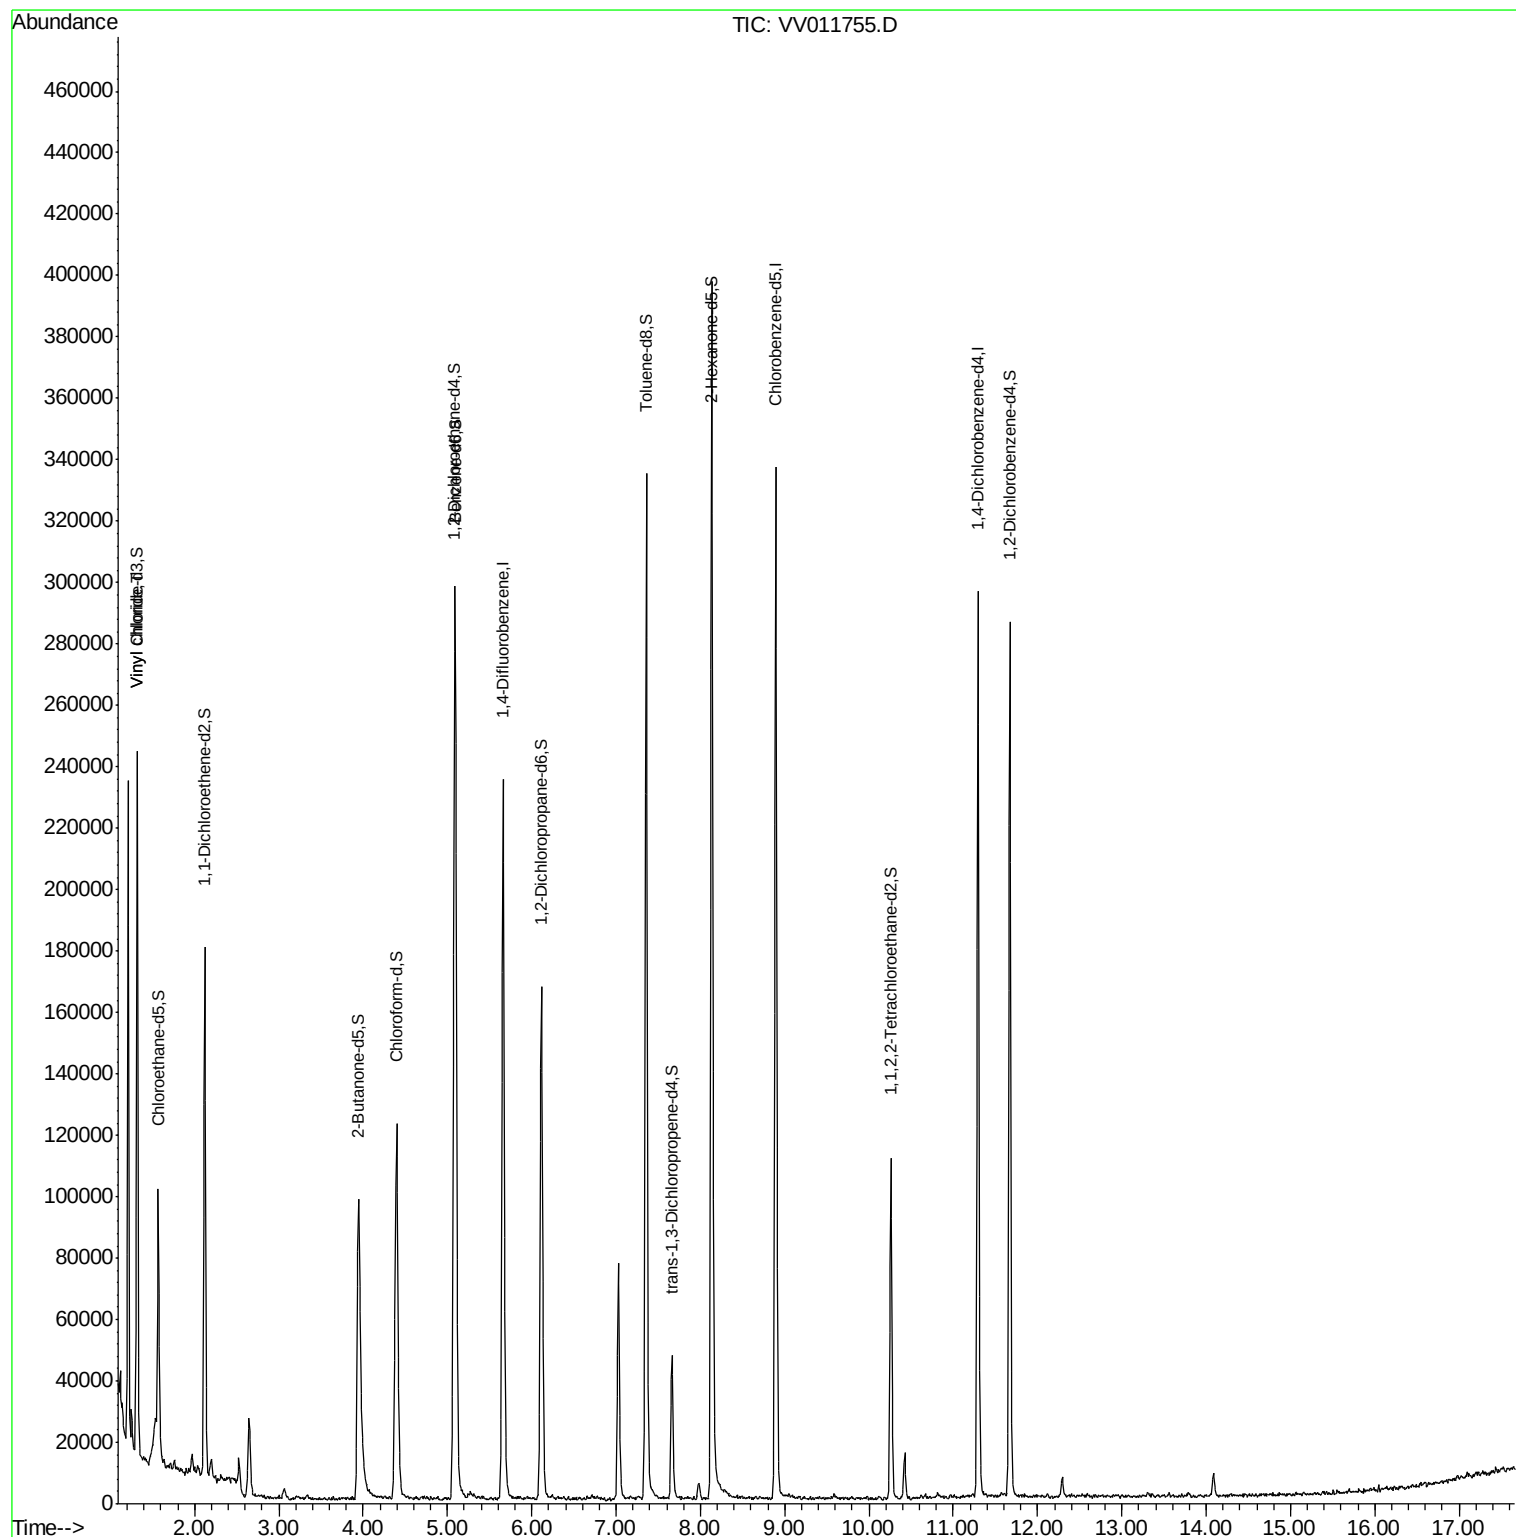

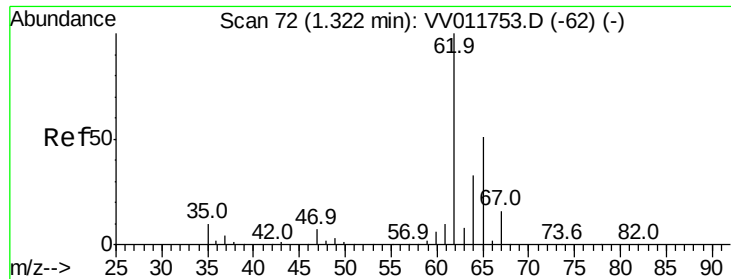

#5
 Vinyl chloride
 Concen: 5.466 ug/L
 RT: 1.32 min Scan# 72
 Delta R.T. -0.00 min
 Lab File: VV011755.D
 Acq: 26 Jun 2019 11:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCP7DL

Tot Ion: 62 Resp: 92035
 Ion Ratio Lower Upper
 62 100
 64 32.2 24.1 44.7

