


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062619\
 Data File : VV011752.D
 Acq On : 26 Jun 2019 10:07
 Operator : SY/MD
 Sample : BFB57
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB57

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 26 12:11:41 2019

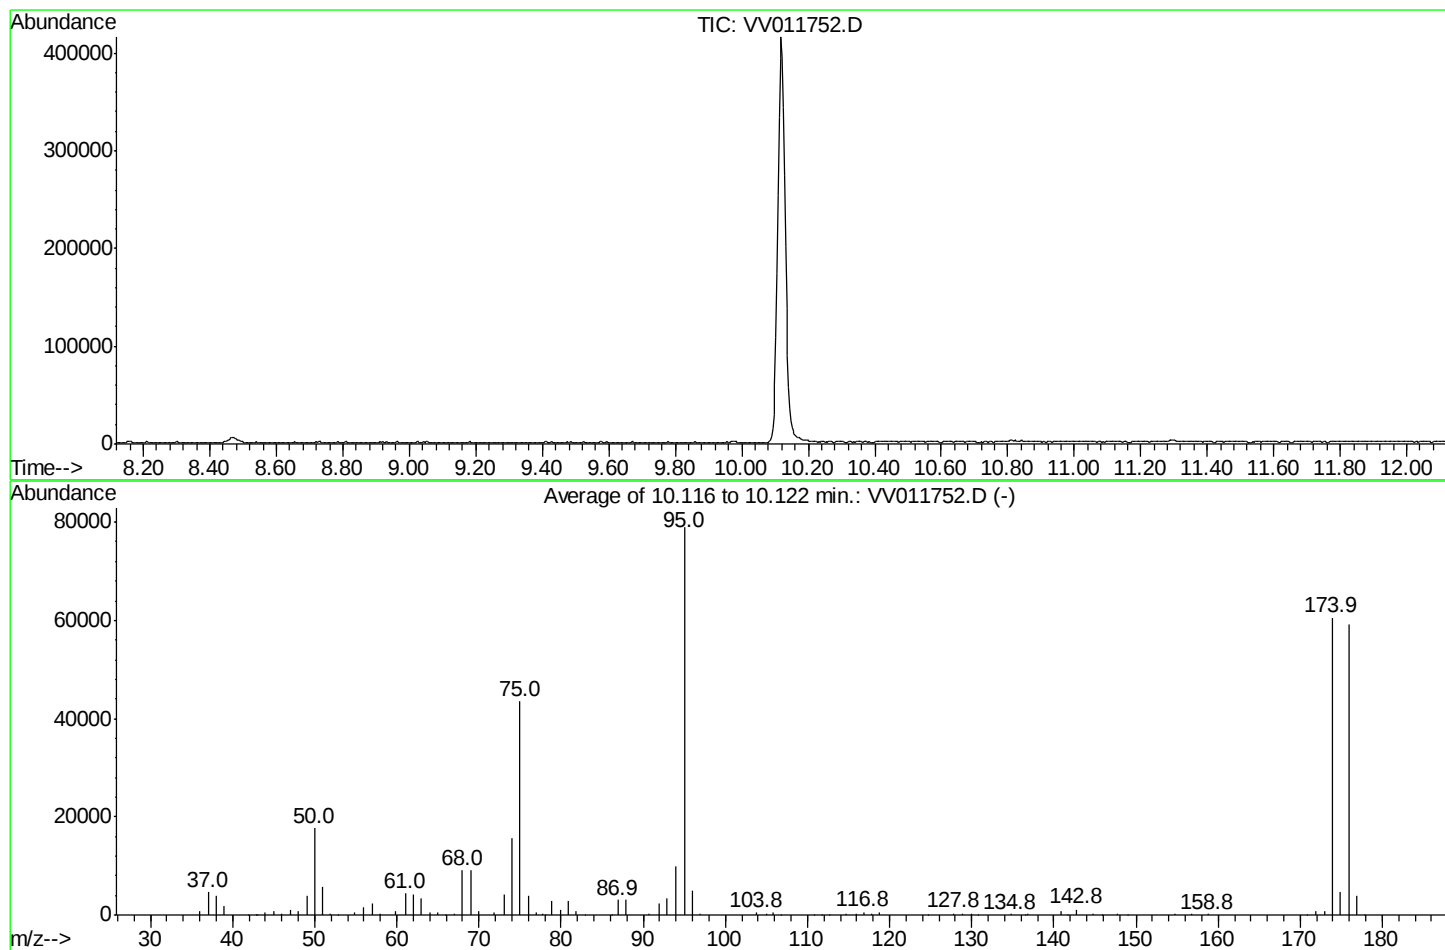

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	17664	PASS
75	95	30	80	55.0	43450	PASS
95	95	100	100	100.0	78954	PASS
96	95	5	9	6.4	5026	PASS
173	174	0.00	2	1.5	884	PASS
174	95	50	120	76.7	60520	PASS
175	174	5	9	7.8	4727	PASS
176	174	95	101	97.7	59154	PASS
177	176	5	9	6.6	3932	PASS

Scan 2793 (10.071 min): VV011752.D
BFB57

m/z	Abundance
36.20	105.0
39.00	119.0
39.80	410.0
40.90	125.0
43.90	449.0
46.40	102.0
77.20	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	774.0
37.00	4517.0
38.00	3916.0
39.00	1902.0
39.90	397.0
42.80	105.0
43.90	1126.0
44.90	796.0
45.90	177.0
47.00	1264.0
47.90	701.0
49.00	3844.0
50.00	17736.0
51.00	5705.0
51.90	209.0
52.80	115.0
54.90	393.0
56.00	1564.0
57.00	2395.0
58.00	206.0
59.90	908.0
61.00	4451.0
62.00	4312.0
62.90	3404.0
64.00	469.0
65.00	602.0
65.90	104.0
67.00	191.0
68.00	8967.0
69.00	8982.0
69.90	776.0
71.90	525.0
73.00	4058.0
74.00	15752.0
75.00	43040.0
76.00	4054.0
76.90	513.0
78.00	342.0
78.90	2992.0
79.90	990.0
80.90	2738.0
81.90	825.0
82.80	145.0
86.90	3057.0
87.90	2877.0
90.70	403.0
91.90	2390.0
92.90	3468.0
94.00	10169.0
95.00	77000.0
96.00	5127.0
97.00	224.0
103.80	393.0
104.90	159.0
105.80	394.0
106.70	162.0
110.80	107.0
111.70	105.0
112.60	137.0
114.70	139.0
115.90	344.0
116.80	618.0
117.90	333.0
118.80	542.0
127.90	349.0
128.90	140.0
129.90	309.0
130.80	107.0
134.80	210.0
136.50	140.0
136.90	173.0
140.80	760.0
141.70	116.0
142.80	1078.0
144.90	177.0
146.00	106.0
147.80	277.0
149.00	117.0
154.80	149.0
156.80	155.0
158.70	186.0
170.80	127.0
171.90	657.0
173.00	865.0
173.90	57584.0
174.90	4656.0
175.90	56704.0
176.90	3872.0
177.80	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	842.0
37.00	4849.0
38.00	3989.0
39.00	1928.0
39.90	384.0
42.80	109.0
43.90	1113.0
45.00	803.0
45.90	170.0
47.00	1173.0
47.90	705.0
49.00	4079.0
50.00	18232.0
51.00	5858.0
51.90	262.0
52.80	118.0
54.90	441.0
56.00	1711.0
57.00	2568.0
57.90	237.0
59.90	811.0
61.00	4487.0
62.00	4466.0
63.00	3436.0
64.00	465.0
65.00	650.0
67.00	200.0
68.00	9410.0
69.00	9455.0
69.90	792.0
71.90	519.0
73.00	4269.0
74.00	16293.0
75.00	44856.0
76.00	4066.0
77.00	500.0
77.70	383.0
78.90	2957.0
79.90	989.0
80.90	2929.0
81.80	865.0
82.80	131.0
86.90	3238.0
87.90	3104.0
90.70	404.0
91.90	2425.0
92.90	3468.0
94.00	10307.0
95.00	81912.0
96.00	5083.0
96.90	222.0
103.80	465.0
105.00	146.0
105.80	402.0
106.70	138.0
110.70	118.0
111.80	120.0
112.60	132.0
114.70	153.0
115.90	336.0
116.80	618.0
117.80	344.0
118.80	539.0
124.60	123.0
127.80	400.0
128.90	226.0
129.90	310.0
130.70	138.0
134.80	216.0
136.50	148.0
136.90	178.0
140.80	829.0
141.60	137.0
142.80	1166.0
144.80	253.0
145.90	140.0
147.80	327.0
149.10	123.0
154.70	164.0
156.90	186.0
158.70	207.0
170.90	123.0
171.90	761.0
173.00	863.0
173.90	62744.0
174.90	4887.0
175.90	61488.0
176.90	4067.0
177.80	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	887.0
37.00	4637.0
38.00	3767.0
39.00	1749.0
39.90	380.0
41.90	103.0
43.00	109.0
43.90	1006.0
45.00	785.0
45.90	167.0
47.00	979.0
48.00	613.0
49.00	3832.0
50.00	17024.0
51.00	5409.0
51.90	295.0
52.80	124.0
54.90	407.0
56.00	1624.0
57.00	2426.0
57.80	224.0
59.90	761.0
61.00	4084.0
62.00	4081.0
63.00	3143.0
64.00	454.0
65.00	601.0
67.00	213.0
68.00	8808.0
69.00	9034.0
69.90	760.0
71.90	472.0
73.00	4087.0
74.00	15062.0
75.00	42456.0
76.00	3731.0
77.00	463.0
77.70	383.0
78.90	2765.0
79.90	899.0
80.90	2898.0
81.90	787.0
82.90	114.0
86.10	142.0
86.90	3094.0
87.90	3067.0
90.70	379.0
91.90	2333.0
92.90	3226.0
94.00	9567.0
95.00	77952.0
96.00	4869.0
96.90	227.0
103.80	517.0
105.00	153.0
105.90	406.0
110.70	121.0
111.80	123.0
114.80	150.0
115.90	298.0
116.80	609.0
117.80	365.0
118.70	467.0
124.60	126.0
127.80	408.0
128.90	243.0
129.90	313.0
130.70	140.0
134.80	210.0
136.60	130.0
136.90	162.0
140.90	847.0
142.80	1113.0
144.80	275.0
145.80	145.0
147.80	316.0
154.70	187.0
156.90	200.0
158.80	174.0
171.80	783.0
173.00	925.0
173.90	61232.0
174.90	4638.0
175.90	59272.0
176.90	3858.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57