
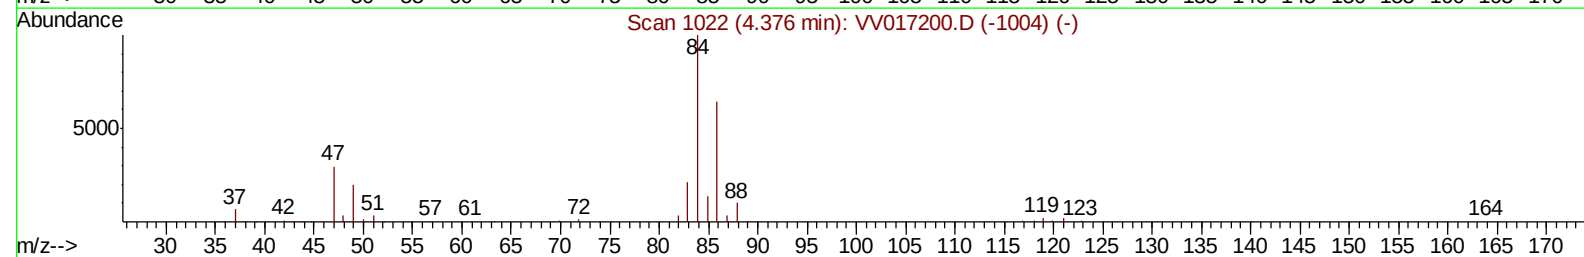
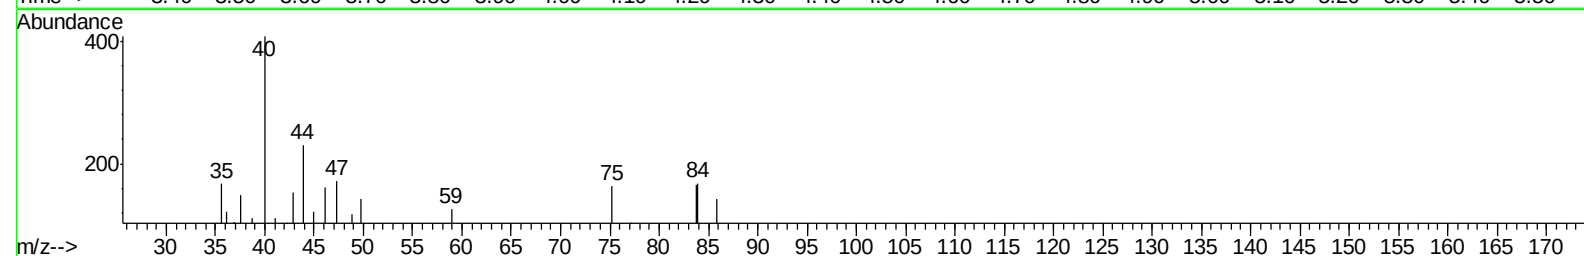


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017210.D
 Acq On : 27 Jun 2020 03:30
 Operator : SY/MD
 Sample : L3132-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Quant Time: Jun 27 05:04:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 27 03:31:05 2020
 Response via : Initial Calibration

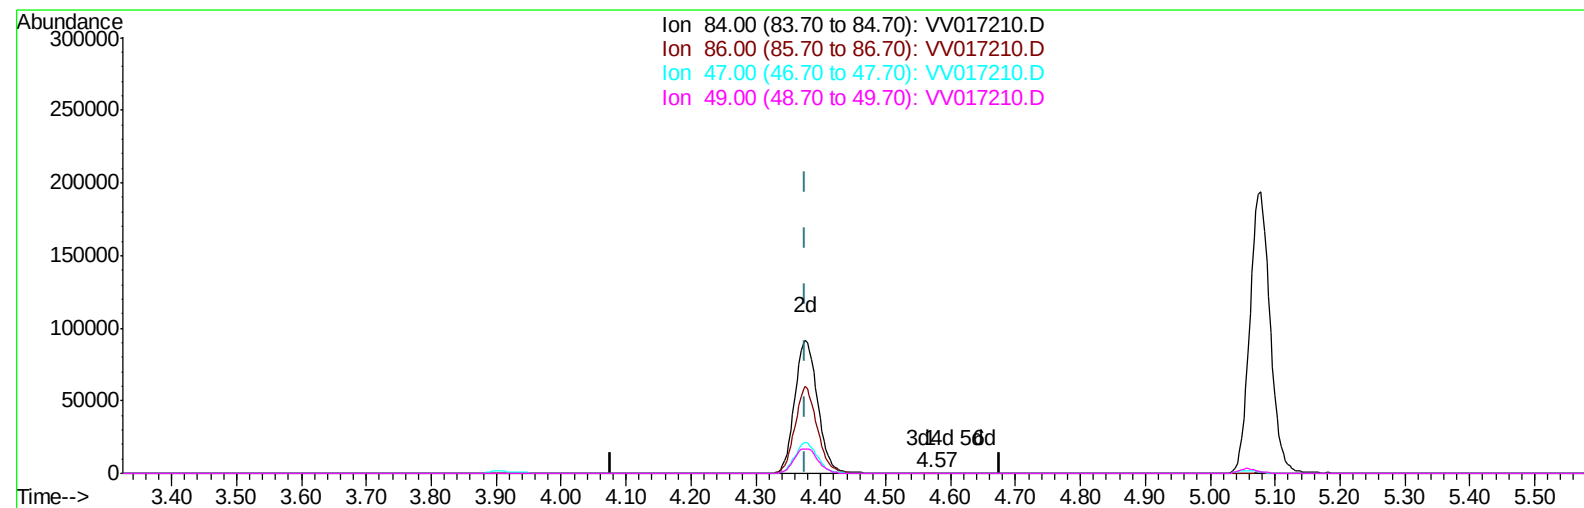

TIC: VV017210.D

(24) Chloroform-d (S)

4.569min (+0.193) 0.05ug/L

response 225

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	50.22
47.00	44.50	47.56
49.00	27.40	33.33