
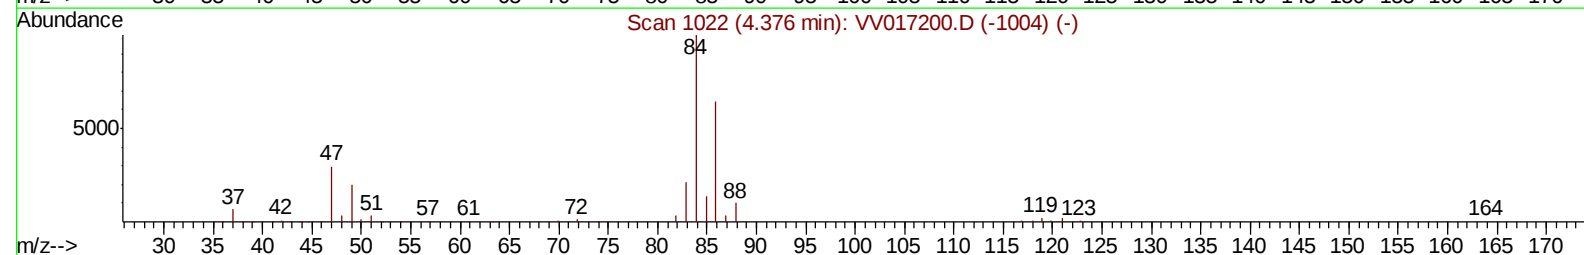
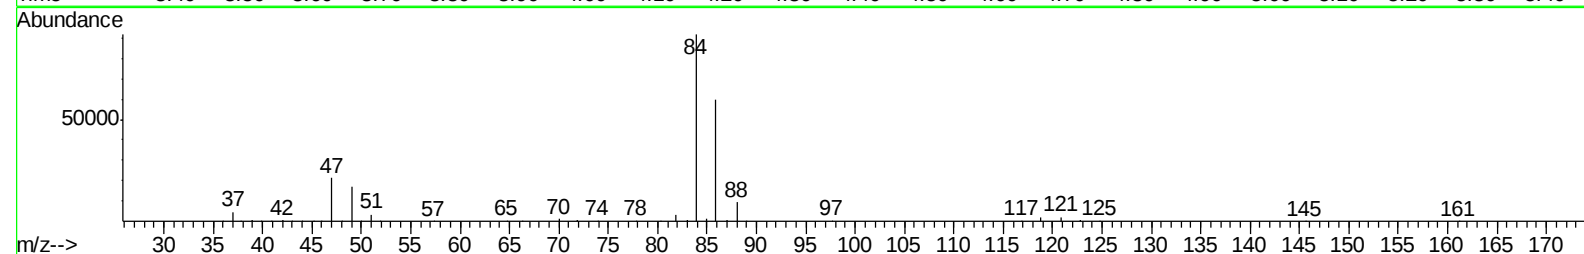


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017210.D
Acq On : 27 Jun 2020 03:30
Operator : SY/MD
Sample : L3132-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Jun 27 05:04:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 27 03:31:05 2020
Response via : Initial Calibration

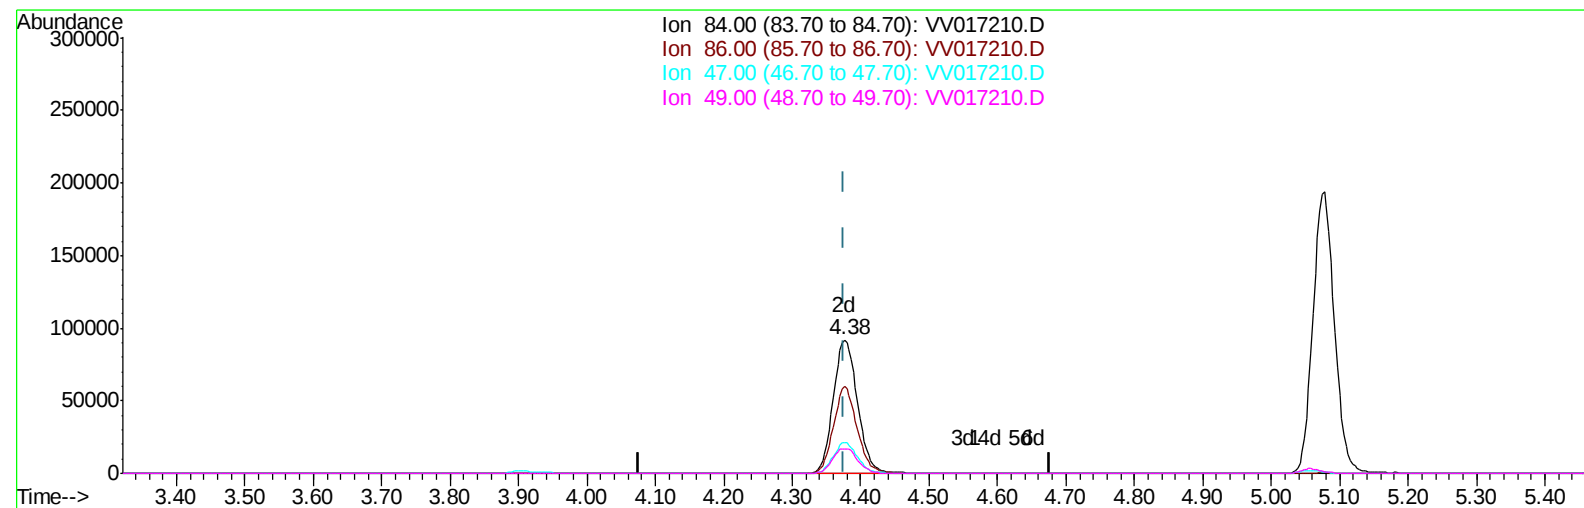

TIC: VV017210.D

(24) Chloroform-d (S)

4.376min (-0.000) 45.49ug/L m

response 224983

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	0.05#
47.00	44.50	0.05#
49.00	27.40	0.03#