


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017213.D
Acq On : 27 Jun 2020 04:39
Operator : SY/MD
Sample : L3132-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0Y32

Manual Integrations
APPROVED

MMDadoda
6/30/2020 1:57:34 PM

Quant Time: Jun 27 05:27:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 27 03:31:05 2020
Response via : Initial Calibration

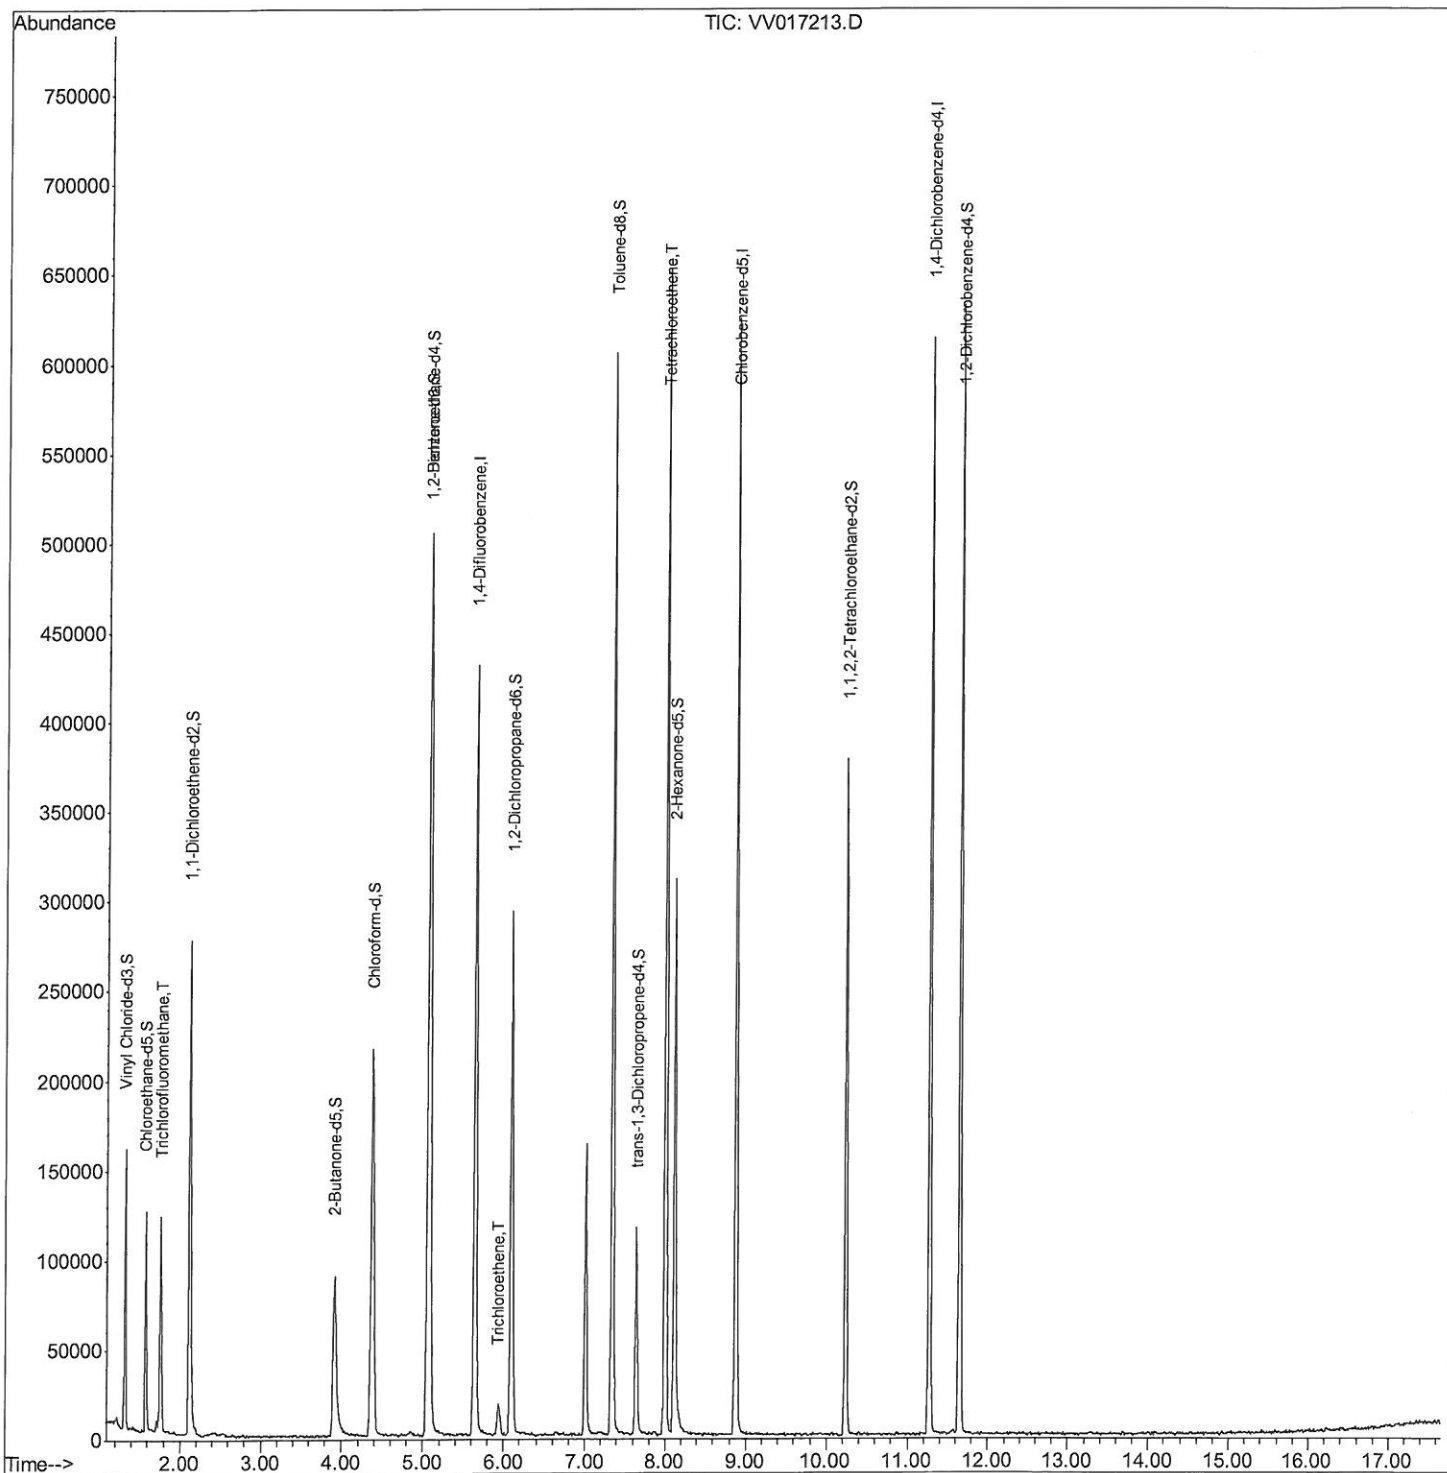

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017213.D
 Acq On : 27 Jun 2020 04:39
 Operator : SY/MD
 Sample : L3132-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0Y32

Manual Integrations
APPROVED

MMDadoda
 6/30/2020 1:57:34 PM

Quant Time: Jun 27 05:04:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 27 03:31:05 2020
 Response via : Initial Calibration

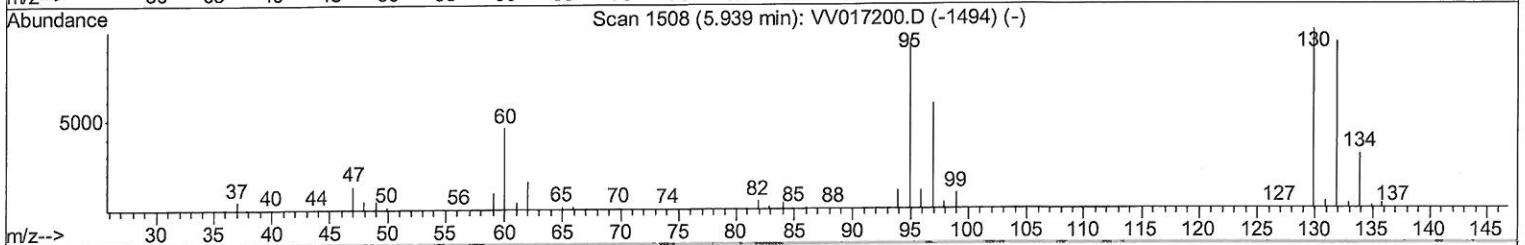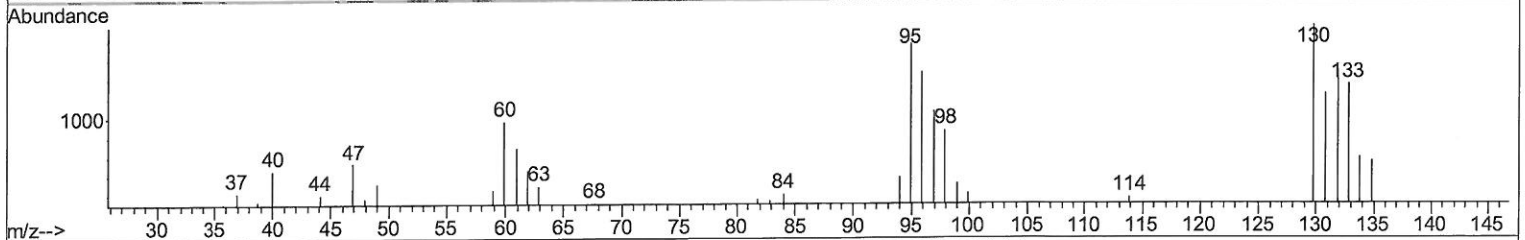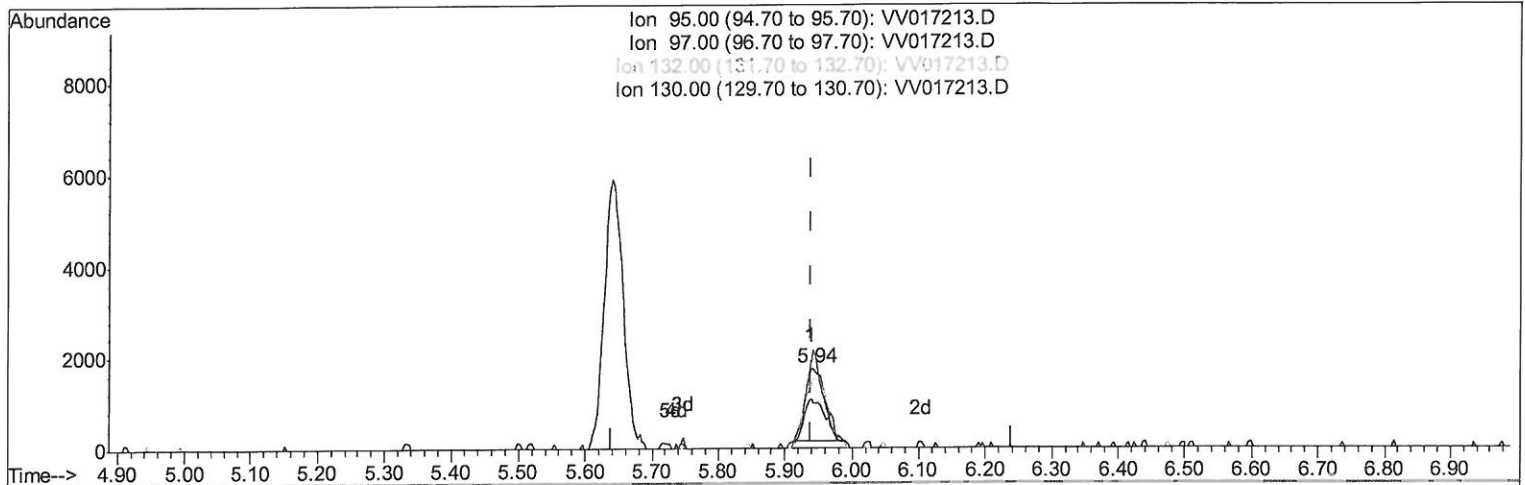

TIC: VV017213.D

(34) Trichloroethene (T)
 5.939min (-0.000) 1.23ug/L
 response 3194

Ion	Exp%	Act%
95.00	100	100
97.00	63.30	60.77
132.00	97.00	84.18
130.00	103.20	111.08

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017213.D
Acq On : 27 Jun 2020 04:39
Operator : SY/MD
Sample : L3132-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0Y32

Manual Integrations
APPROVED

MMDadoda
6/30/2020 1:57:34 PM

Quant Time: Jun 27 05:04:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 27 03:31:05 2020
Response via : Initial Calibration

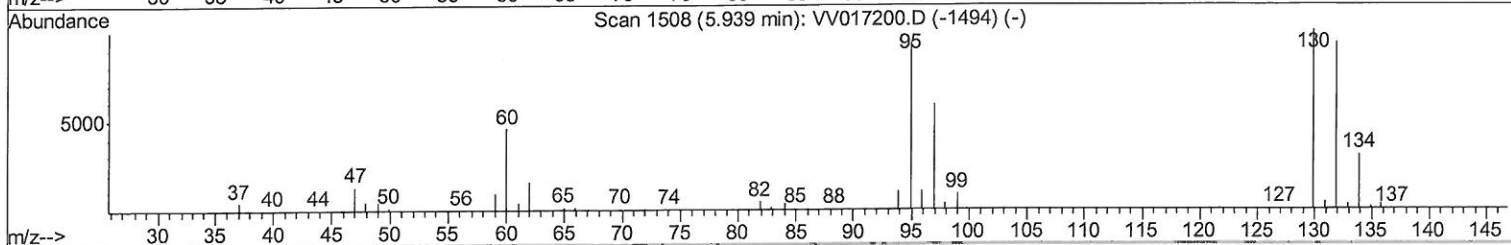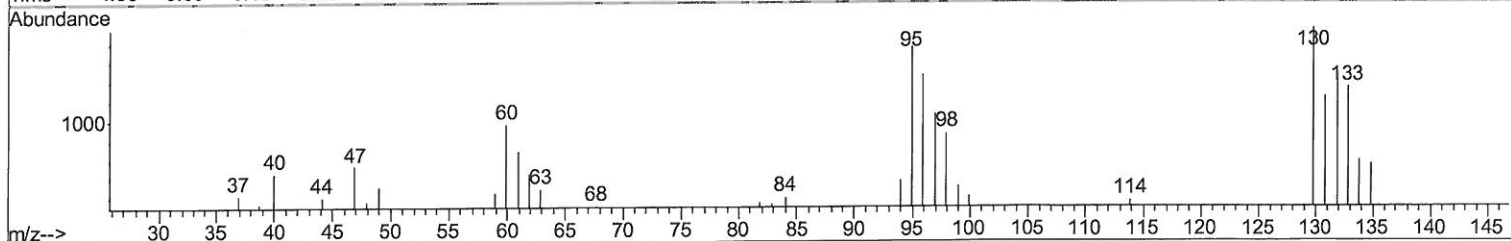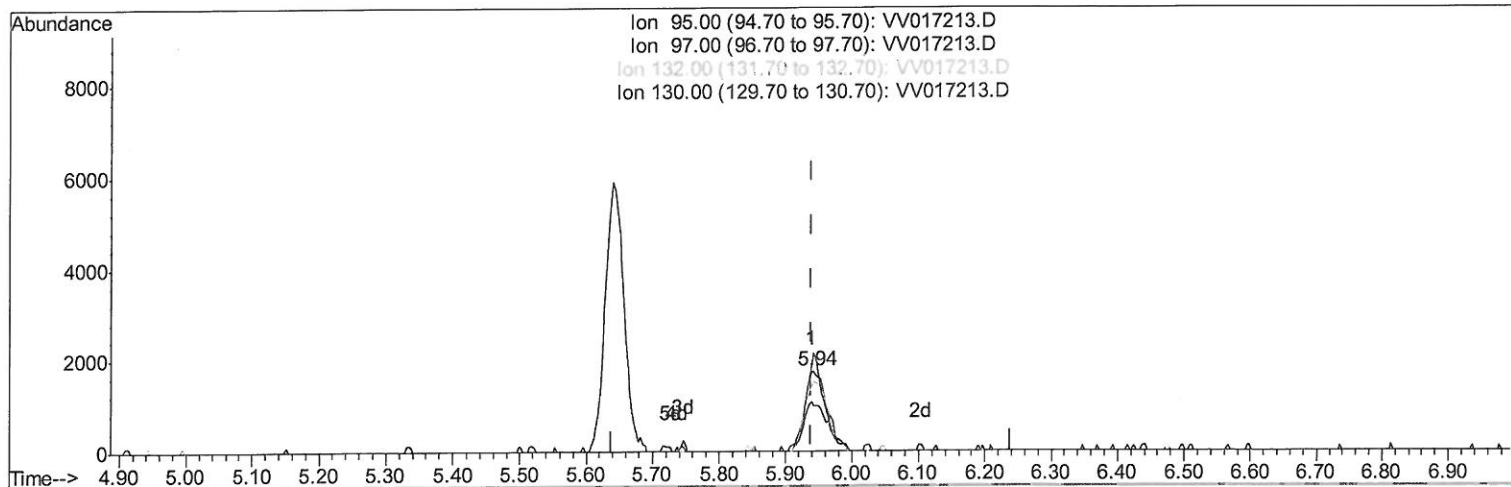

TIC: VV017213.D

(34) Trichloroethene (T)

5.939min (-0.000) 1.51ug/L m

response 3928

Ion	Exp%	Act%
95.00	100	100
97.00	63.30	60.77
132.00	97.00	84.18
130.00	103.20	111.08

MD
06/30/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017213.D
 Acq On : 27 Jun 2020 04:39
 Operator : SY/MD
 Sample : L3132-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y32

Manual Integrations
 APPROVED

MMDadoda
 6/30/2020 1:57:34 PM

Quant Time: Jun 27 05:27:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 27 03:31:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	347975	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	327447	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	150979	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	94453	38.47	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.94%		
7) Chloroethane-d5	1.58	69	69240	47.00	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.00%		
11) 1,1-Dichloroethene-d2	2.12	63	146849	35.62	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.24%		
21) 2-Butanone-d5	3.91	46	153473	84.45	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.45%		
24) Chloroform-d	4.38	84	218428	43.75	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.50%		
26) 1,2-Dichloroethane-d4	5.06	65	159085	46.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.68%		
32) Benzene-d6	5.08	84	411592	43.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.20%		
36) 1,2-Dichloropropane-d6	6.09	67	123003	41.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.60%		
41) Toluene-d8	7.34	98	376796	43.50	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.00%		
43) trans-1,3-Dichloropropene-	7.64	79	62955	41.08	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.16%		
47) 2-Hexanone-d5	8.11	63	101495	79.12	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.12%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	161992	41.59	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.18%		
64) 1,2-Dichlorobenzene-d4	11.65	152	154451	47.94	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.88%		

Target Compounds					Ovalue
9) Trichlorofluoromethane	1.77	101	70886	19.093 ug/L	99
34) Trichloroethene	5.94	95	3928m	1.512 ug/L	
46) Tetrachloroethene	8.00	164	139605	68.315 ug/L	98

MD
 06/30/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed