

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017185.D
 Acq On : 26 Jun 2020 16:40
 Operator : SY/MD
 Sample : L3103-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q10

Quant Time: Jun 27 00:50:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 27 00:23:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	282811	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	268634	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	125364	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	94345	47.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.56%
7) Chloroethane-d5	1.58	69	68068	56.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	113.70%
11) 1,1-Dichloroethene-d2	2.12	63	144741	43.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.38%
21) 2-Butanone-d5	3.91	46	140526	95.14	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.14%
24) Chloroform-d	4.38	84	211660	52.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.32%
26) 1,2-Dichloroethane-d4	5.06	65	151692	54.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.92%
32) Benzene-d6	5.08	84	400612	51.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.46%
36) 1,2-Dichloropropane-d6	6.09	67	117651	48.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.48%
41) Toluene-d8	7.34	98	354640	49.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.82%
43) trans-1,3-Dichloropropene-	7.64	79	60976	48.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.00%
47) 2-Hexanone-d5	8.11	63	94342	89.65	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.65%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	154774	48.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.88%
64) 1,2-Dichlorobenzene-d4	11.65	152	145920	54.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.08%


Target Compounds					Ovalue
13) Acetone	2.19	43	15818	16.254 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017185.D
Acq On : 26 Jun 2020 16:40
Operator : SY/MD
Sample : L3103-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q10

Quant Time: Jun 27 00:50:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 27 00:23:55 2020
Response via : Initial Calibration

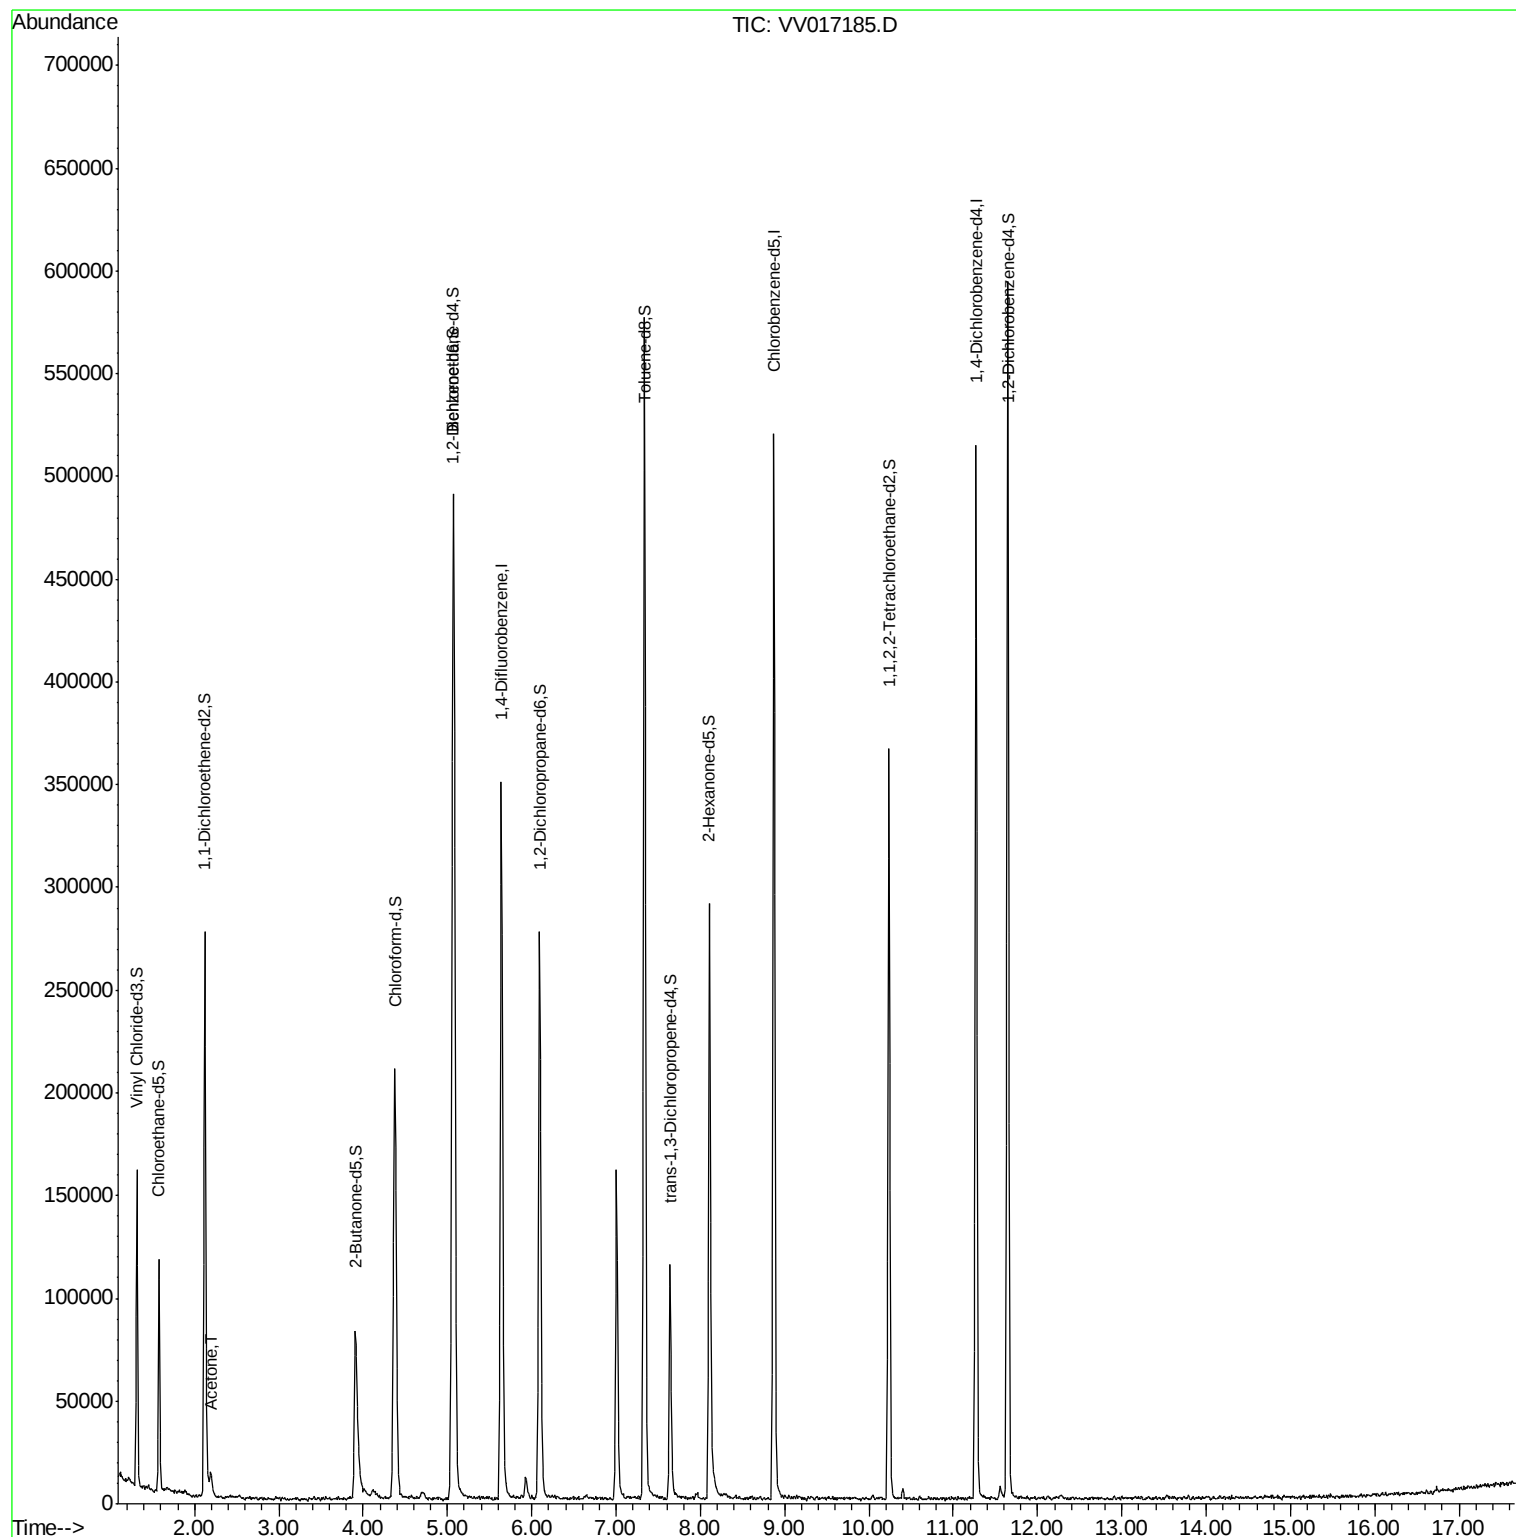

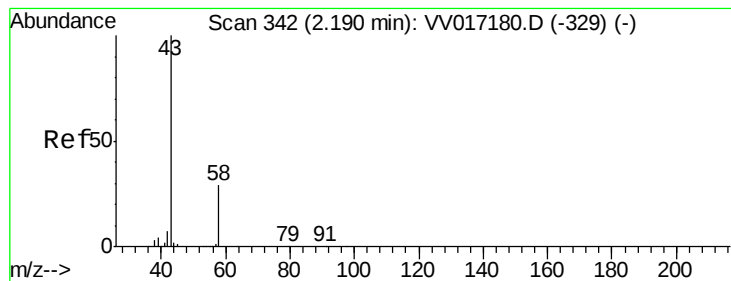

#13

Acetone

Concen: 16.254 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV017185.D

Acq: 26 Jun 2020 16:40

Instrument :
MSVOA_V
ClientSampleId :
F9Q10

Tot Ion: 43 Resp: 15818

Ion Ratio Lower Upper

43 100

58 30.9 0.0 55.2

