

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017202.D
 Acq On : 27 Jun 2020 00:24
 Operator : SY/MD
 Sample : L3118-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F81

Quant Time: Jun 27 03:48:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 27 03:31:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	351394	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	332521	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	154315	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	97499	39.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.64%
7) Chloroethane-d5	1.58	69	65257	43.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.72%
11) 1,1-Dichloroethene-d2	2.12	63	150110	36.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.10%
21) 2-Butanone-d5	3.90	46	148562	80.95	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.95%
24) Chloroform-d	4.38	84	219923	43.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.24%
26) 1,2-Dichloroethane-d4	5.06	65	156795	45.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.44%
32) Benzene-d6	5.08	84	415415	43.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.68%
36) 1,2-Dichloropropane-d6	6.09	67	124339	41.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.22%
41) Toluene-d8	7.34	98	381017	43.32	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.64%
43) trans-1,3-Dichloropropene-	7.64	79	62680	40.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.56%
47) 2-Hexanone-d5	8.11	63	96356	73.97	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	73.97%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	161904	40.93	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.86%
64) 1,2-Dichlorobenzene-d4	11.65	152	154885	47.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.06%


Target Compounds					Ovalue
13) Acetone	2.19	43	7514	6.214 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017202.D
Acq On : 27 Jun 2020 00:24
Operator : SY/MD
Sample : L3118-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F81

Quant Time: Jun 27 03:48:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 27 03:31:05 2020
Response via : Initial Calibration

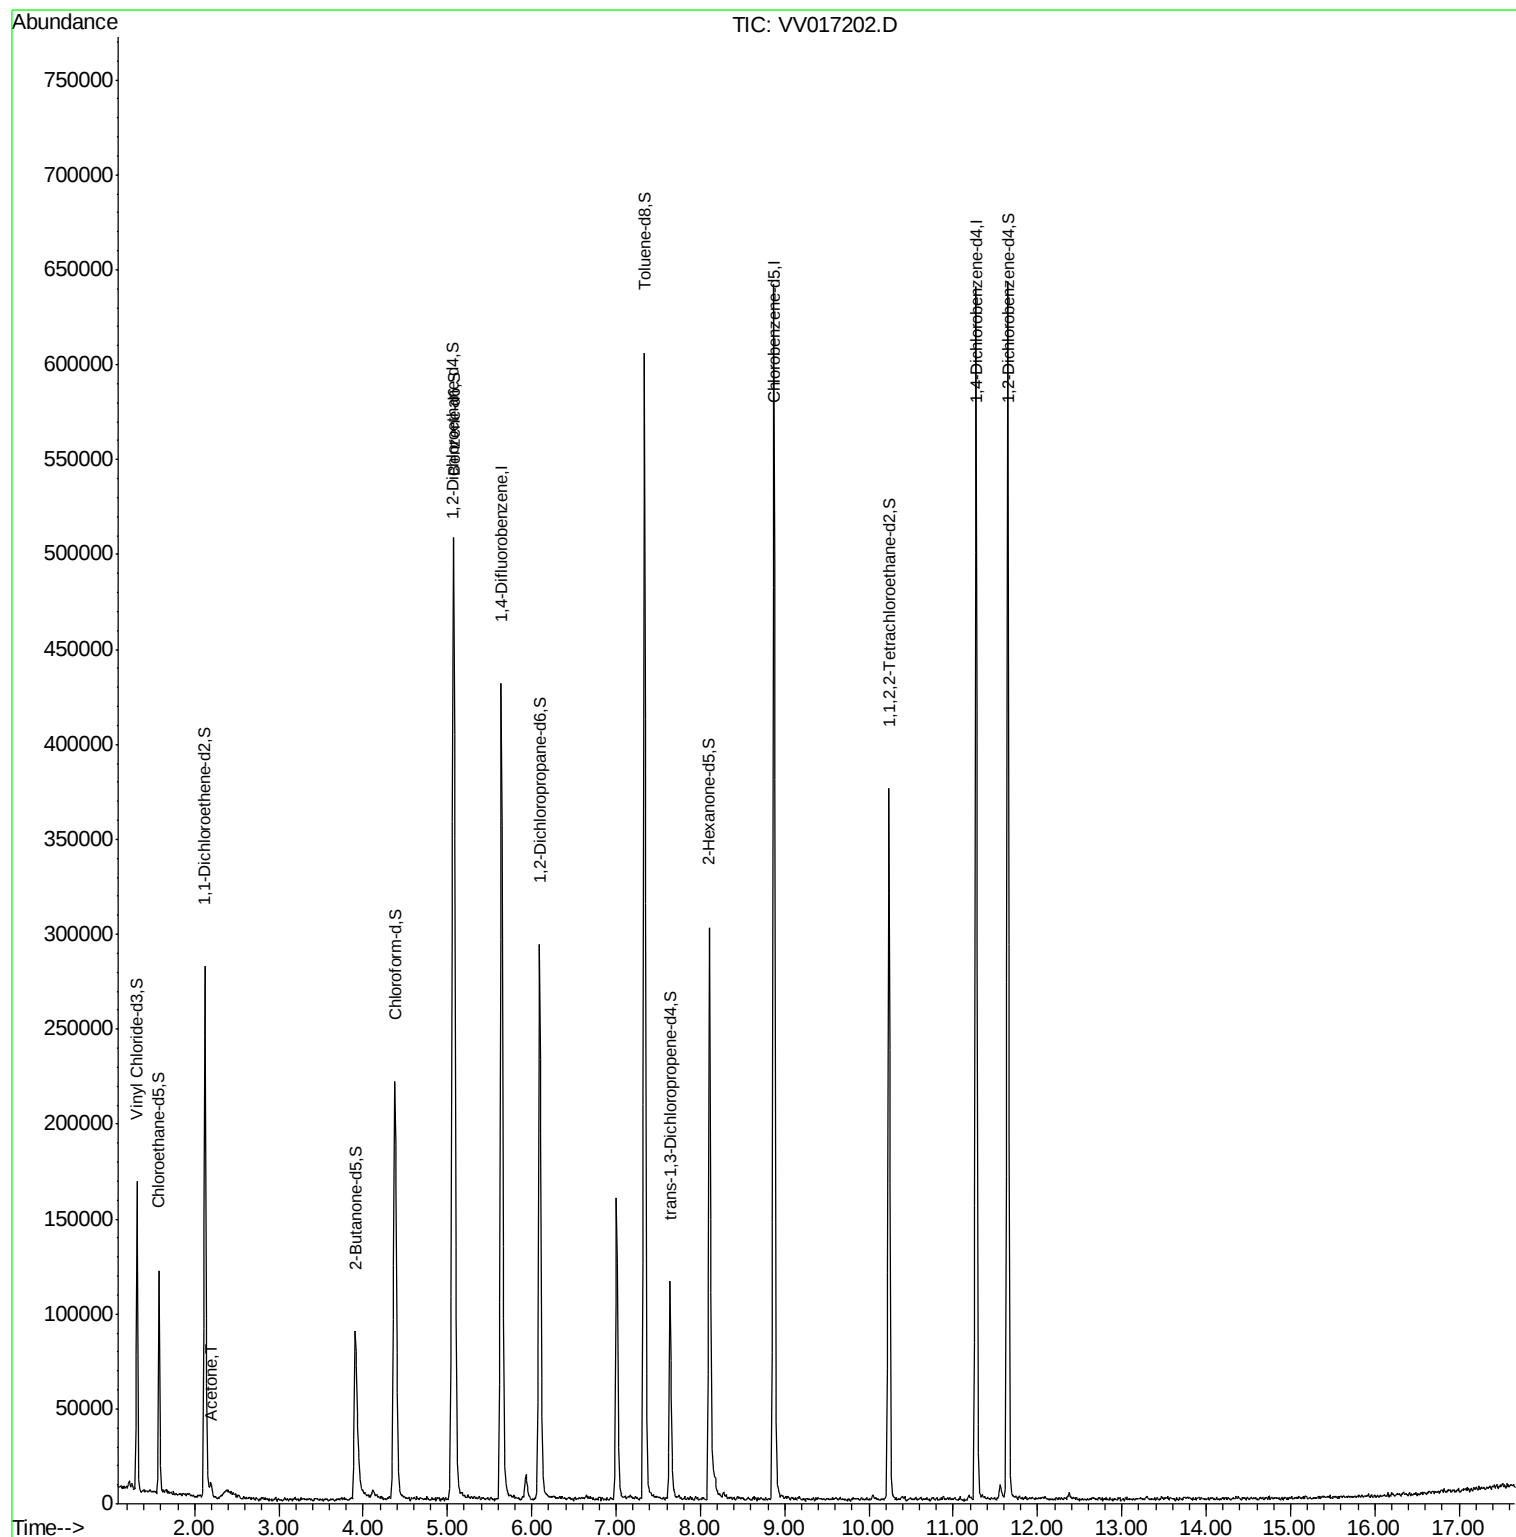

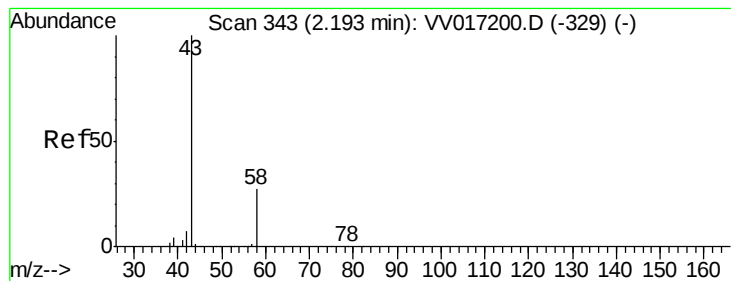

#13

Acetone

Concen: 6.214 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV017202.D

Acq: 27 Jun 2020 00:24

Instrument :
MSVOA_V
ClientSampleId :
C0F81

Tot Ion: 43 Resp: 7514

Ion Ratio Lower Upper

43 100

58 35.4 0.0 55.2

