

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017181.D
 Acq On : 26 Jun 2020 15:06
 Operator : SY/MD
 Sample : VV0626WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	179060	185078	13.30%	1.747%
2	1.579	145	152	160	rVB	125426	139413	10.02%	1.316%
3	2.119	310	320	340	rVB	312445	464952	33.42%	4.388%
4	2.434	416	418	421	rVB2	1226	694	0.05%	0.007%
5	2.669	488	491	493	rBV4	1554	1021	0.07%	0.010%
6	2.849	544	547	549	rVB4	1856	922	0.07%	0.009%
7	2.862	549	551	552	rBV2	642	210	0.02%	0.002%
8	2.888	558	559	561	rBV2	977	505	0.04%	0.005%
9	2.917	567	568	569	rBV	780	281	0.02%	0.003%
10	3.071	614	616	618	rVB3	1212	444	0.03%	0.004%
11	3.158	640	643	644	rBV3	1712	979	0.07%	0.009%
12	3.254	671	673	676	rBV3	909	490	0.04%	0.005%
13	3.293	682	685	686	rBV3	1100	552	0.04%	0.005%
14	3.389	709	715	716	rBV4	1354	1423	0.10%	0.013%
15	3.524	754	757	760	rBV4	1103	941	0.07%	0.009%
16	3.579	769	774	776	rBV4	2084	1816	0.13%	0.017%
17	3.692	806	809	810	rBV2	883	494	0.04%	0.005%
18	3.904	864	875	905	rBV	95886	274780	19.75%	2.593%
19	4.142	946	949	951	rBV4	1897	1036	0.07%	0.010%
20	4.370	1006	1020	1043	rBV2	227580	555455	39.93%	5.242%
21	4.601	1090	1092	1095	rBV3	1050	628	0.05%	0.006%
22	4.801	1152	1154	1157	rBV4	1529	787	0.06%	0.007%
23	4.865	1172	1174	1177	rVB4	2009	961	0.07%	0.009%
24	5.068	1219	1237	1261	rBV3	538977	1391200	100.00%	13.128%
25	5.547	1383	1386	1387	rBV2	1429	771	0.06%	0.007%
26	5.637	1401	1414	1441	rBV	432047	864686	62.15%	8.160%
27	5.830	1468	1474	1480	rBV7	2255	2959	0.21%	0.028%
28	5.929	1496	1505	1514	rBV10	8585	17003	1.22%	0.160%
29	5.990	1522	1524	1526	rBV2	1187	549	0.04%	0.005%
30	6.090	1543	1555	1576	rVB	304897	612179	44.00%	5.777%
31	6.441	1663	1664	1666	rBV2	955	286	0.02%	0.003%
32	6.502	1681	1683	1684	rBV2	1183	472	0.03%	0.004%
33	6.634	1720	1724	1726	rBV4	1464	1317	0.09%	0.012%
34	6.949	1818	1822	1826	rBV4	1311	1142	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017181.D
 Acq On : 26 Jun 2020 15:06
 Operator : SY/MD
 Sample : VV0626WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.003	1828	1839	1858	rVV	177394	320572	23.04%	3.025%
36	7.335	1930	1942	1963	rBV	659126	1121439	80.61%	10.583%
37	7.515	1995	1998	2002	rBV5	1638	1353	0.10%	0.013%
38	7.640	2027	2037	2056	rBV	129318	224084	16.11%	2.115%
39	7.817	2090	2092	2095	rVB3	1338	622	0.04%	0.006%
40	8.106	2172	2182	2211	rBV	329403	596012	42.84%	5.624%
41	8.521	2308	2311	2315	rBV5	1215	1016	0.07%	0.010%
42	8.691	2362	2364	2365	rBV2	1160	524	0.04%	0.005%
43	8.871	2408	2420	2441	rBV	651242	1041594	74.87%	9.829%
44	9.296	2549	2552	2555	rBV4	1604	1074	0.08%	0.010%
45	9.466	2603	2605	2609	rBV4	1377	1075	0.08%	0.010%
46	9.749	2692	2693	2696	rBV2	1097	527	0.04%	0.005%
47	9.781	2701	2703	2705	rBV3	990	436	0.03%	0.004%
48	9.865	2726	2729	2731	rBV3	1409	737	0.05%	0.007%
49	9.907	2739	2742	2748	rVB7	1678	1382	0.10%	0.013%
50	10.064	2789	2791	2797	rVB5	1576	1256	0.09%	0.012%
51	10.125	2808	2810	2812	rBV2	1282	557	0.04%	0.005%
52	10.235	2833	2844	2858	rBV	410467	643835	46.28%	6.076%
53	10.392	2891	2893	2902	rVB6	1645	1604	0.12%	0.015%
54	10.428	2902	2904	2906	rBV3	1538	758	0.05%	0.007%
55	10.473	2916	2918	2920	rBV3	760	409	0.03%	0.004%
56	10.794	3016	3018	3021	rBV4	1294	807	0.06%	0.008%
57	10.830	3027	3029	3031	rVB3	1571	630	0.05%	0.006%
58	10.981	3074	3076	3079	rBV2	893	405	0.03%	0.004%
59	11.074	3099	3105	3108	rBV4	1777	2053	0.15%	0.019%
60	11.270	3155	3166	3184	rBV	653780	1006459	72.34%	9.498%
61	11.482	3230	3232	3235	rBV3	1252	859	0.06%	0.008%
62	11.547	3250	3252	3254	rBV2	1179	371	0.03%	0.004%
63	11.646	3271	3283	3300	rBV	697360	1079991	77.63%	10.191%
64	11.797	3327	3330	3332	rBV4	1857	1159	0.08%	0.011%
65	11.900	3360	3362	3363	rBV2	1071	384	0.03%	0.004%
66	11.948	3375	3377	3378	rBV	1312	498	0.04%	0.005%
67	12.013	3395	3397	3402	rVB3	1192	642	0.05%	0.006%
68	12.074	3412	3416	3419	rBV4	1593	1558	0.11%	0.015%
69	12.167	3440	3445	3447	rBV4	1735	1376	0.10%	0.013%
70	12.665	3596	3600	3601	rBV2	2791	1961	0.14%	0.019%
71	12.955	3688	3690	3693	rBV3	1220	974	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017181.D
Acq On : 26 Jun 2020 15:06
Operator : SY/MD
Sample : VV0626WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Title : VOC Analysis

72	13.055	3718	3721	3724	rVB4	1748	982	0.07%	0.009%
73	13.071	3724	3726	3727	rBV	617	224	0.02%	0.002%
74	13.080	3727	3729	3730	rBV2	1406	680	0.05%	0.006%
75	13.186	3758	3762	3765	rBV4	1593	1637	0.12%	0.015%
76	13.276	3786	3790	3791	rBV3	2919	1920	0.14%	0.018%
77	13.617	3892	3896	3897	rBV3	1436	934	0.07%	0.009%
78	13.723	3925	3929	3932	rBV5	1546	1256	0.09%	0.012%
79	14.029	4022	4024	4025	rBV2	1371	679	0.05%	0.006%
80	14.173	4068	4069	4071	rBV	845	462	0.03%	0.004%
81	14.984	4318	4321	4323	rBV2	1329	817	0.06%	0.008%


Sum of corrected areas: 10597010

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017181.D
Acq On : 26 Jun 2020 15:06
Operator : SY/MD
Sample : VV0626WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

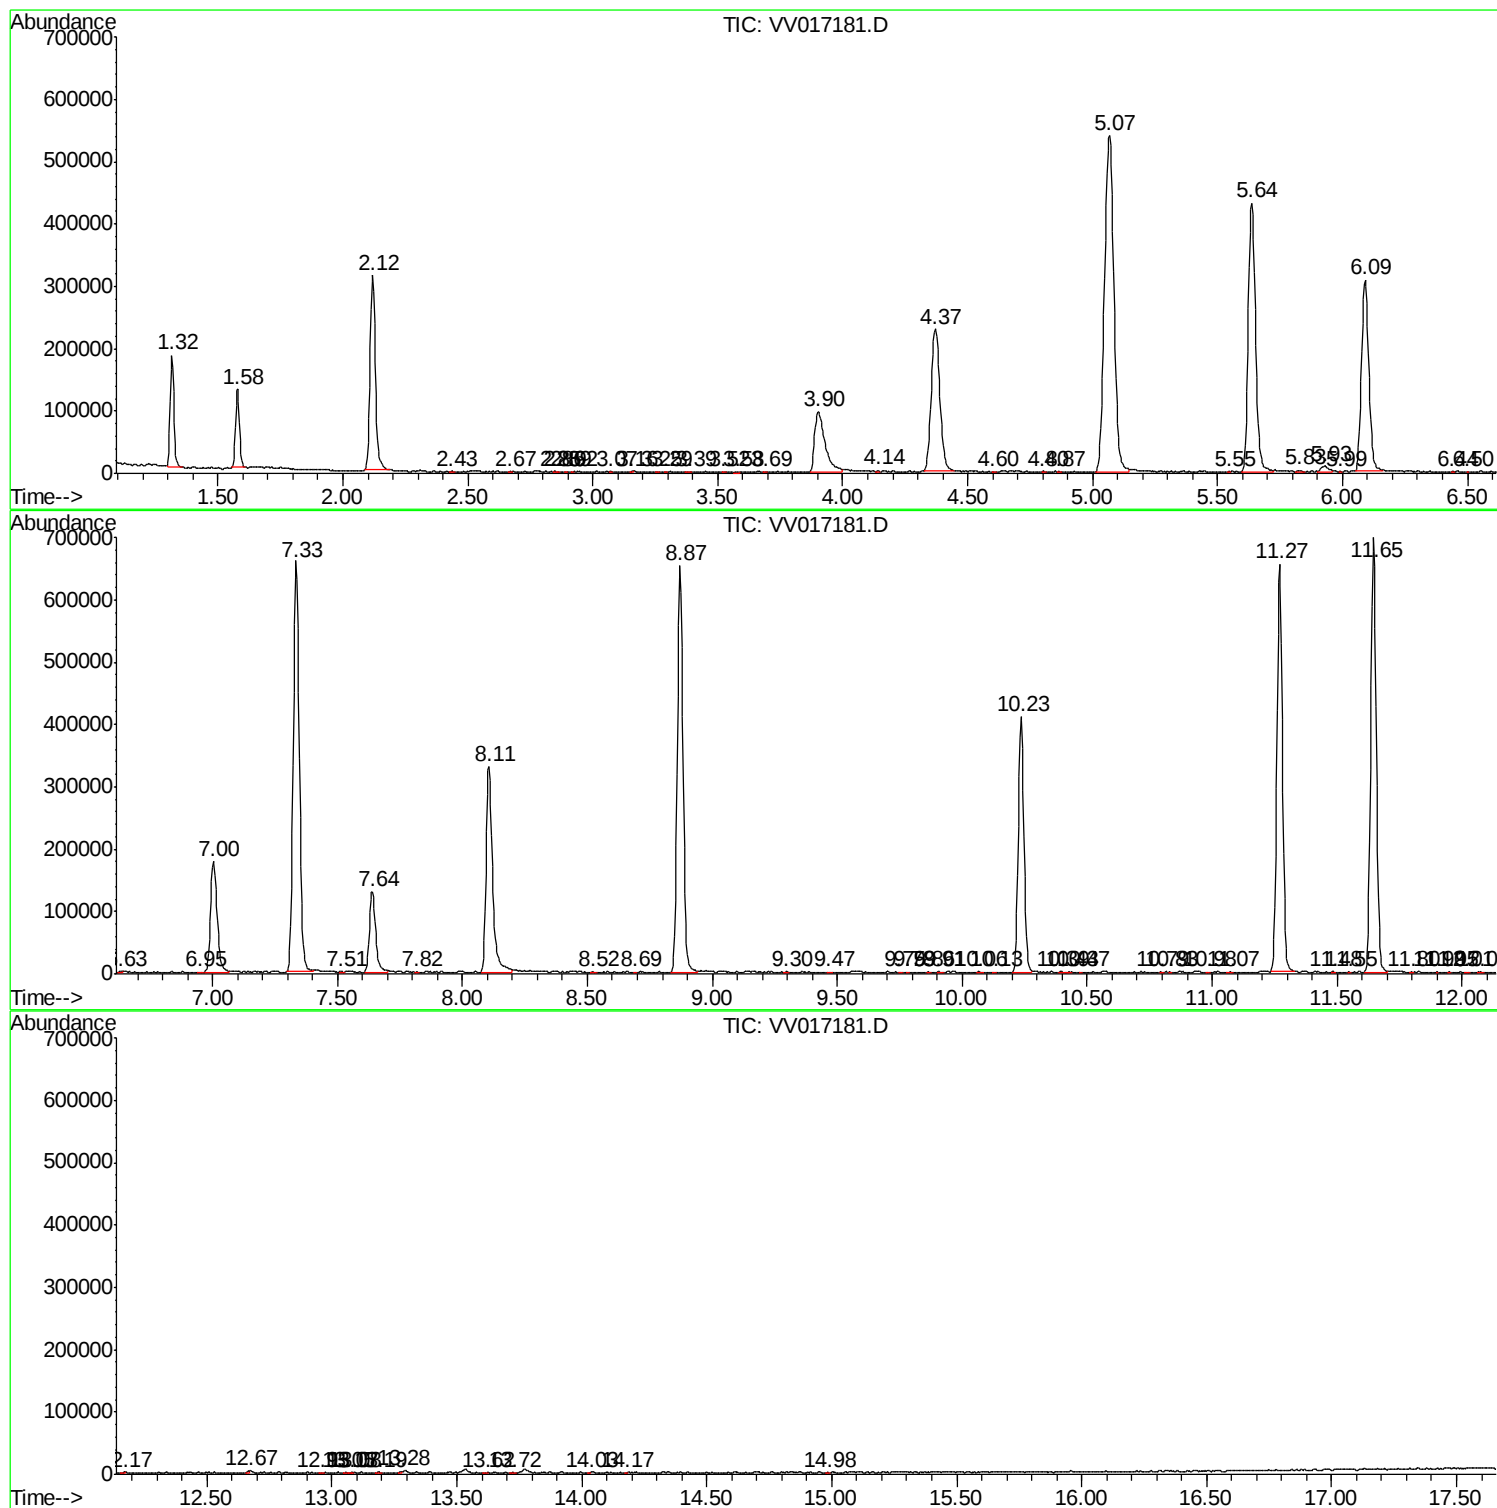

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017181.D
Acq On : 26 Jun 2020 15:06
Operator : SY/MD
Sample : VV0626WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017181.D
Acq On : 26 Jun 2020 15:06
Operator : SY/MD
Sample : VV0626WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
