

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017182.D
 Acq On : 26 Jun 2020 15:30
 Operator : SY/MD
 Sample : L3103-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	168536	175350	11.93%	1.667%
2	1.579	146	152	163	rVB	127809	138727	9.44%	1.319%
3	2.122	311	321	342	rVB	295992	447509	30.44%	4.254%
4	2.592	465	467	473	rVB5	1511	936	0.06%	0.009%
5	2.630	474	479	481	rBV4	1517	1295	0.09%	0.012%
6	2.736	510	512	515	rBV3	1043	489	0.03%	0.005%
7	2.897	560	562	564	rBV2	1256	577	0.04%	0.005%
8	2.994	590	592	594	rBV3	991	400	0.03%	0.004%
9	3.058	609	612	617	rBV6	1483	1840	0.13%	0.017%
10	3.167	642	646	648	rBV4	1311	1132	0.08%	0.011%
11	3.373	707	710	712	rVB3	1406	735	0.05%	0.007%
12	3.386	712	714	716	rBV2	814	279	0.02%	0.003%
13	3.457	734	736	740	rBV4	1057	576	0.04%	0.005%
14	3.521	754	756	758	rBV2	1160	539	0.04%	0.005%
15	3.534	758	760	763	rVV4	1170	694	0.05%	0.007%
16	3.585	774	776	778	rBV3	1632	926	0.06%	0.009%
17	3.614	783	785	786	rBV	643	246	0.02%	0.002%
18	3.650	794	796	798	rBV3	1013	401	0.03%	0.004%
19	3.698	808	811	812	rBV2	1066	451	0.03%	0.004%
20	3.814	846	847	850	rBV3	978	616	0.04%	0.006%
21	3.904	864	875	904	rBV	103055	300416	20.43%	2.856%
22	4.228	974	976	979	rBV4	1206	756	0.05%	0.007%
23	4.289	993	995	1000	rVB5	2676	2228	0.15%	0.021%
24	4.373	1000	1021	1051	rBV2	252248	638694	43.44%	6.072%
25	5.071	1220	1238	1262	rBV2	570687	1470304	100.00%	13.978%
26	5.640	1403	1415	1436	rBV	358587	709627	48.26%	6.746%
27	6.093	1541	1556	1583	rBV	324827	668919	45.50%	6.359%
28	6.421	1656	1658	1662	rBV5	1206	678	0.05%	0.006%
29	6.579	1705	1707	1709	rBV	1323	684	0.05%	0.007%
30	6.640	1719	1726	1729	rBV6	2593	3286	0.22%	0.031%
31	6.871	1795	1798	1800	rBV3	1656	1325	0.09%	0.013%
32	6.910	1808	1810	1813	rBV3	1284	731	0.05%	0.007%
33	6.942	1818	1820	1822	rBV3	1278	683	0.05%	0.006%
34	7.006	1827	1840	1860	rBV	191467	342186	23.27%	3.253%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017182.D
 Acq On : 26 Jun 2020 15:30
 Operator : SY/MD
 Sample : L3103-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.286	1925	1927	1929	rBV3	1061	456	0.03%	0.004%
36	7.338	1931	1943	1960	rVV	665972	1154857	78.55%	10.979%
37	7.595	2021	2023	2026	rBV3	1504	951	0.06%	0.009%
38	7.640	2027	2037	2050	rVV	139366	232846	15.84%	2.214%
39	7.778	2078	2080	2081	rBV2	1433	497	0.03%	0.005%
40	7.903	2118	2119	2120	rBV	822	309	0.02%	0.003%
41	7.958	2128	2136	2146	rBV2	13757	23683	1.61%	0.225%
42	8.106	2171	2182	2212	rBV	360142	650725	44.26%	6.186%
43	8.672	2356	2358	2361	rVB4	1329	432	0.03%	0.004%
44	8.688	2361	2363	2364	rBV2	852	458	0.03%	0.004%
45	8.871	2408	2420	2440	rBV	556453	897183	61.02%	8.529%
46	9.100	2489	2491	2493	rVB2	1390	511	0.03%	0.005%
47	9.376	2576	2577	2581	rVB4	1528	830	0.06%	0.008%
48	9.411	2583	2588	2590	rBV5	998	930	0.06%	0.009%
49	9.482	2608	2610	2612	rBV3	726	277	0.02%	0.003%
50	9.569	2632	2637	2639	rBV3	1964	1731	0.12%	0.016%
51	9.701	2673	2678	2681	rBV4	1932	1681	0.11%	0.016%
52	10.183	2826	2828	2829	rBV2	1156	490	0.03%	0.005%
53	10.238	2834	2845	2859	rVV	432722	675244	45.93%	6.419%
54	10.344	2876	2878	2880	rVB3	937	318	0.02%	0.003%
55	10.453	2910	2912	2913	rBV2	853	391	0.03%	0.004%
56	10.553	2941	2943	2945	rBV3	1249	740	0.05%	0.007%
57	10.595	2955	2956	2963	rVB7	1423	1158	0.08%	0.011%
58	10.627	2963	2966	2970	rVB4	1345	911	0.06%	0.009%
59	10.646	2970	2972	2977	rBV4	1463	1177	0.08%	0.011%
60	10.685	2982	2984	2986	rBV2	1254	574	0.04%	0.005%
61	10.720	2991	2995	2996	rBV5	777	417	0.03%	0.004%
62	10.759	3005	3007	3009	rBV3	1122	637	0.04%	0.006%
63	10.797	3017	3019	3021	rBV3	846	384	0.03%	0.004%
64	10.845	3032	3034	3038	rBV5	1466	1133	0.08%	0.011%
65	11.270	3155	3166	3187	rBV	538081	828707	56.36%	7.878%
66	11.534	3247	3248	3252	rBV3	808	483	0.03%	0.005%
67	11.646	3271	3283	3298	rBV	707128	1100713	74.86%	10.464%
68	11.923	3364	3369	3371	rBV5	1150	832	0.06%	0.008%
69	11.932	3371	3372	3373	rVV	947	255	0.02%	0.002%
70	11.952	3376	3378	3380	rBV3	1029	565	0.04%	0.005%
71	12.109	3424	3427	3428	rBV3	988	434	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017182.D
 Acq On : 26 Jun 2020 15:30
 Operator : SY/MD
 Sample : L3103-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.177	3446	3448	3452	rBV3	1321	1031	0.07%	0.010%
73	12.347	3499	3501	3505	rBV3	926	505	0.03%	0.005%
74	12.437	3527	3529	3532	rBV3	1160	910	0.06%	0.009%
75	12.604	3579	3581	3582	rBV2	669	211	0.01%	0.002%
76	12.640	3590	3592	3593	rBV2	1222	376	0.03%	0.004%
77	12.710	3613	3614	3617	rBV3	1012	366	0.02%	0.003%
78	12.826	3648	3650	3652	rBV3	904	417	0.03%	0.004%
79	12.874	3663	3665	3671	rBV6	1381	868	0.06%	0.008%
80	12.945	3683	3687	3690	rBV5	1330	1104	0.08%	0.010%
81	13.000	3702	3704	3706	rBV3	925	564	0.04%	0.005%
82	13.096	3732	3734	3736	rBV3	922	474	0.03%	0.005%
83	13.251	3777	3782	3783	rBV3	1535	1172	0.08%	0.011%
84	13.360	3813	3816	3819	rBV4	1339	740	0.05%	0.007%
85	13.382	3821	3823	3828	rVB2	1753	1294	0.09%	0.012%
86	13.411	3828	3832	3835	rBV4	1385	1483	0.10%	0.014%
87	13.447	3839	3843	3846	rBV4	968	841	0.06%	0.008%
88	13.488	3853	3856	3858	rBV3	883	403	0.03%	0.004%
89	13.633	3899	3901	3903	rBV3	720	381	0.03%	0.004%
90	13.685	3916	3917	3918	rBV	771	230	0.02%	0.002%
91	13.755	3936	3939	3940	rBV3	1674	845	0.06%	0.008%
92	13.935	3993	3995	4000	rBV5	1311	678	0.05%	0.006%
93	14.115	4049	4051	4052	rBV2	1094	430	0.03%	0.004%
94	14.160	4063	4065	4070	rBV6	1331	1196	0.08%	0.011%
95	14.479	4163	4164	4166	rVB2	1400	378	0.03%	0.004%
96	14.492	4166	4168	4170	rBV3	1089	610	0.04%	0.006%
97	14.871	4284	4286	4289	rBV2	1104	618	0.04%	0.006%
98	15.402	4449	4451	4454	rBV3	1315	971	0.07%	0.009%
99	15.488	4475	4478	4479	rBV3	1436	788	0.05%	0.007%
100	15.623	4518	4520	4522	rBV2	1495	836	0.06%	0.008%


Sum of corrected areas: 10518875

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017182.D
Acq On : 26 Jun 2020 15:30
Operator : SY/MD
Sample : L3103-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

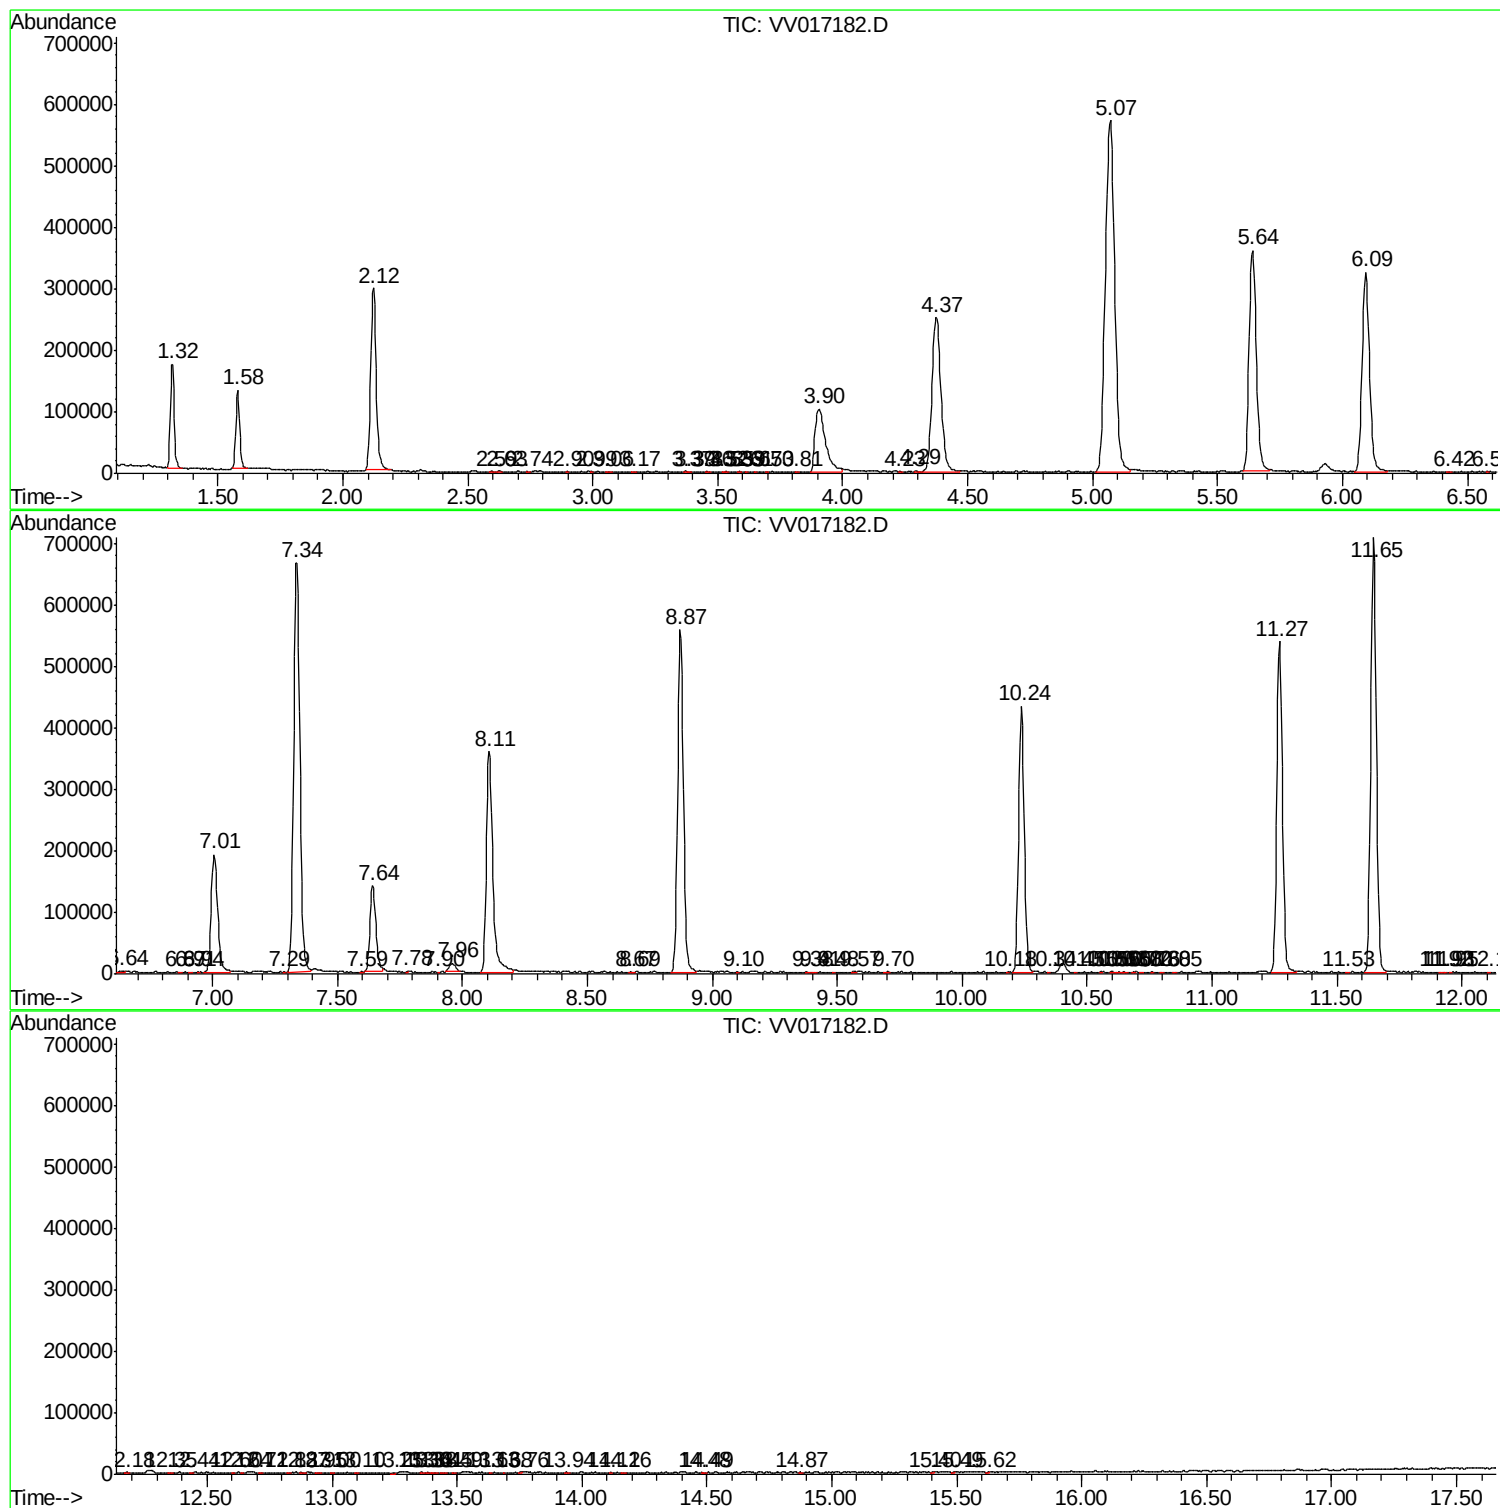

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017182.D
Acq On : 26 Jun 2020 15:30
Operator : SY/MD
Sample : L3103-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017182.D
Acq On : 26 Jun 2020 15:30
Operator : SY/MD
Sample : L3103-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
