

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017183.D
 Acq On : 26 Jun 2020 15:54
 Operator : SY/MD
 Sample : L3103-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	154332	158815	12.90%	1.561%
2	1.579	145	152	165	rVB	110541	122069	9.92%	1.200%
3	2.123	311	321	334	rBV	271557	406371	33.01%	3.994%
4	2.618	472	475	478	rBV5	2138	1503	0.12%	0.015%
5	2.679	490	494	497	rBV5	972	716	0.06%	0.007%
6	2.692	497	498	503	rBV4	1002	655	0.05%	0.006%
7	3.049	607	609	611	rBV3	1720	959	0.08%	0.009%
8	3.139	635	637	644	rVB7	1086	875	0.07%	0.009%
9	3.283	680	682	684	rBV3	1243	714	0.06%	0.007%
10	3.418	722	724	728	rVB4	1606	872	0.07%	0.009%
11	3.447	728	733	735	rBV4	756	597	0.05%	0.006%
12	3.479	740	743	747	rBV5	968	764	0.06%	0.008%
13	3.534	757	760	762	rBV4	1101	595	0.05%	0.006%
14	3.631	786	790	795	rBV5	1244	1035	0.08%	0.010%
15	3.756	825	829	832	rVB5	1335	1187	0.10%	0.012%
16	3.791	836	840	845	rBV7	1252	1053	0.09%	0.010%
17	3.933	864	884	906	rBV4	131616	491584	39.93%	4.832%
18	4.376	1007	1022	1044	rBV	205358	499959	40.61%	4.914%
19	5.071	1221	1238	1262	rBV2	477696	1231118	100.00%	12.101%
20	5.267	1297	1299	1303	rBV3	1205	1038	0.08%	0.010%
21	5.331	1317	1319	1322	rBV4	1585	1111	0.09%	0.011%
22	5.528	1378	1380	1384	rBV5	1459	826	0.07%	0.008%
23	5.640	1403	1415	1440	rBV	414777	821885	66.76%	8.079%
24	5.939	1496	1508	1523	rBV	168891	331066	26.89%	3.254%
25	6.093	1542	1556	1585	rBV	272519	560501	45.53%	5.509%
26	6.576	1703	1706	1710	rVB5	1482	896	0.07%	0.009%
27	6.839	1785	1788	1793	rVB7	2317	1614	0.13%	0.016%
28	6.872	1793	1798	1802	rBV8	1785	1668	0.14%	0.016%
29	7.007	1827	1840	1861	rBV	157632	283112	23.00%	2.783%
30	7.338	1931	1943	1960	rBV	576376	981034	79.69%	9.643%
31	7.527	1998	2002	2007	rBV7	2081	1779	0.14%	0.017%
32	7.569	2010	2015	2020	rVB9	2100	2461	0.20%	0.024%
33	7.595	2020	2023	2025	rBV4	848	730	0.06%	0.007%
34	7.640	2027	2037	2057	rBV	112777	196705	15.98%	1.933%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017183.D
 Acq On : 26 Jun 2020 15:54
 Operator : SY/MD
 Sample : L3103-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.852	2099	2103	2104	rBV3	1515	892	0.07%	0.009%
36	7.904	2118	2119	2124	rBV4	862	735	0.06%	0.007%
37	8.042	2159	2162	2165	rBV4	1193	968	0.08%	0.010%
38	8.106	2172	2182	2207	rBV	282139	496024	40.29%	4.876%
39	8.328	2249	2251	2256	rBV6	1755	1436	0.12%	0.014%
40	8.543	2315	2318	2321	rBV3	1502	983	0.08%	0.010%
41	8.749	2377	2382	2384	rBV3	1525	1116	0.09%	0.011%
42	8.871	2409	2420	2437	rVV	626650	1010784	82.10%	9.935%
43	9.048	2473	2475	2478	rBV4	1265	593	0.05%	0.006%
44	9.164	2507	2511	2512	rBV3	1253	628	0.05%	0.006%
45	9.235	2531	2533	2537	rBV5	1541	873	0.07%	0.009%
46	9.257	2537	2540	2542	rVV4	1031	731	0.06%	0.007%
47	9.334	2561	2564	2567	rBV4	792	583	0.05%	0.006%
48	9.351	2567	2569	2574	rVB5	1153	765	0.06%	0.008%
49	9.373	2574	2576	2581	rBV3	1014	801	0.07%	0.008%
50	9.518	2617	2621	2623	rBV3	1073	907	0.07%	0.009%
51	9.666	2664	2667	2670	rBV3	1338	907	0.07%	0.009%
52	9.756	2691	2695	2696	rBV4	1251	630	0.05%	0.006%
53	9.839	2717	2721	2723	rBV3	1147	672	0.05%	0.007%
54	9.859	2723	2727	2728	rBV3	1102	604	0.05%	0.006%
55	9.875	2728	2732	2736	rBV4	1753	1416	0.12%	0.014%
56	9.958	2755	2758	2761	rVB4	1973	1239	0.10%	0.012%
57	9.987	2761	2767	2769	rBV7	1425	1356	0.11%	0.013%
58	10.087	2796	2798	2802	rVB3	1515	948	0.08%	0.009%
59	10.235	2832	2844	2860	rBV	352885	564359	45.84%	5.547%
60	10.402	2888	2896	2904	rBV3	20211	29508	2.40%	0.290%
61	10.704	2983	2990	2995	rBV9	1932	2059	0.17%	0.020%
62	10.830	3026	3029	3032	rBV5	1028	676	0.05%	0.007%
63	10.859	3036	3038	3041	rVB3	1019	606	0.05%	0.006%
64	10.974	3072	3074	3076	rBV3	1346	613	0.05%	0.006%
65	11.010	3080	3085	3088	rVV5	1106	994	0.08%	0.010%
66	11.048	3095	3097	3100	rBV3	1413	869	0.07%	0.009%
67	11.138	3123	3125	3129	rBV4	1361	828	0.07%	0.008%
68	11.154	3129	3130	3134	rVV4	1363	809	0.07%	0.008%
69	11.270	3155	3166	3182	rBV	624892	954106	77.50%	9.378%
70	11.386	3200	3202	3206	rBV4	1230	635	0.05%	0.006%
71	11.559	3247	3256	3267	rBV4	5790	12518	1.02%	0.123%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017183.D
 Acq On : 26 Jun 2020 15:54
 Operator : SY/MD
 Sample : L3103-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3298	rVV	596312	929408	75.49%	9.135%
73	11.868	3349	3352	3355	rBV4	1866	1373	0.11%	0.013%
74	11.926	3365	3370	3371	rBV4	1269	928	0.08%	0.009%
75	11.932	3371	3372	3378	rVB4	1875	930	0.08%	0.009%
76	12.093	3419	3422	3425	rBV4	1286	835	0.07%	0.008%
77	12.125	3429	3432	3435	rBV4	1722	1317	0.11%	0.013%
78	12.267	3471	3476	3486	rVB4	6593	10863	0.88%	0.107%
79	12.624	3585	3587	3591	rBV4	1826	1658	0.13%	0.016%
80	12.865	3658	3662	3665	rBV4	1206	1151	0.09%	0.011%
81	12.942	3684	3686	3689	rVB3	2064	857	0.07%	0.008%
82	12.968	3689	3694	3698	rBV5	1998	2445	0.20%	0.024%
83	12.987	3698	3700	3704	rVV4	1148	828	0.07%	0.008%
84	13.055	3717	3721	3726	rBV7	1076	1146	0.09%	0.011%
85	13.106	3735	3737	3739	rBV3	1260	640	0.05%	0.006%
86	13.193	3761	3764	3767	rBV3	1420	800	0.06%	0.008%
87	13.373	3817	3820	3821	rBV3	1160	669	0.05%	0.007%
88	13.505	3858	3861	3865	rVB5	1774	1290	0.10%	0.013%
89	13.727	3922	3930	3931	rBV6	1843	1695	0.14%	0.017%
90	13.900	3982	3984	3989	rBV5	1460	809	0.07%	0.008%
91	14.022	4017	4022	4026	rVB4	1912	1666	0.14%	0.016%
92	14.051	4026	4031	4034	rBV6	1482	1333	0.11%	0.013%
93	14.151	4059	4062	4063	rBV3	1276	737	0.06%	0.007%
94	14.247	4089	4092	4095	rBV3	1197	680	0.06%	0.007%
95	14.347	4119	4123	4124	rBV3	1750	1360	0.11%	0.013%
96	14.694	4229	4231	4235	rVB4	1150	665	0.05%	0.007%
97	15.077	4347	4350	4352	rBV2	1218	791	0.06%	0.008%
98	15.299	4416	4419	4423	rBV4	1709	1652	0.13%	0.016%
99	15.482	4474	4476	4480	rBV4	1531	946	0.08%	0.009%
100	15.559	4497	4500	4502	rBV3	1520	1120	0.09%	0.011%


Sum of corrected areas: 10173630

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017183.D
Acq On : 26 Jun 2020 15:54
Operator : SY/MD
Sample : L3103-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

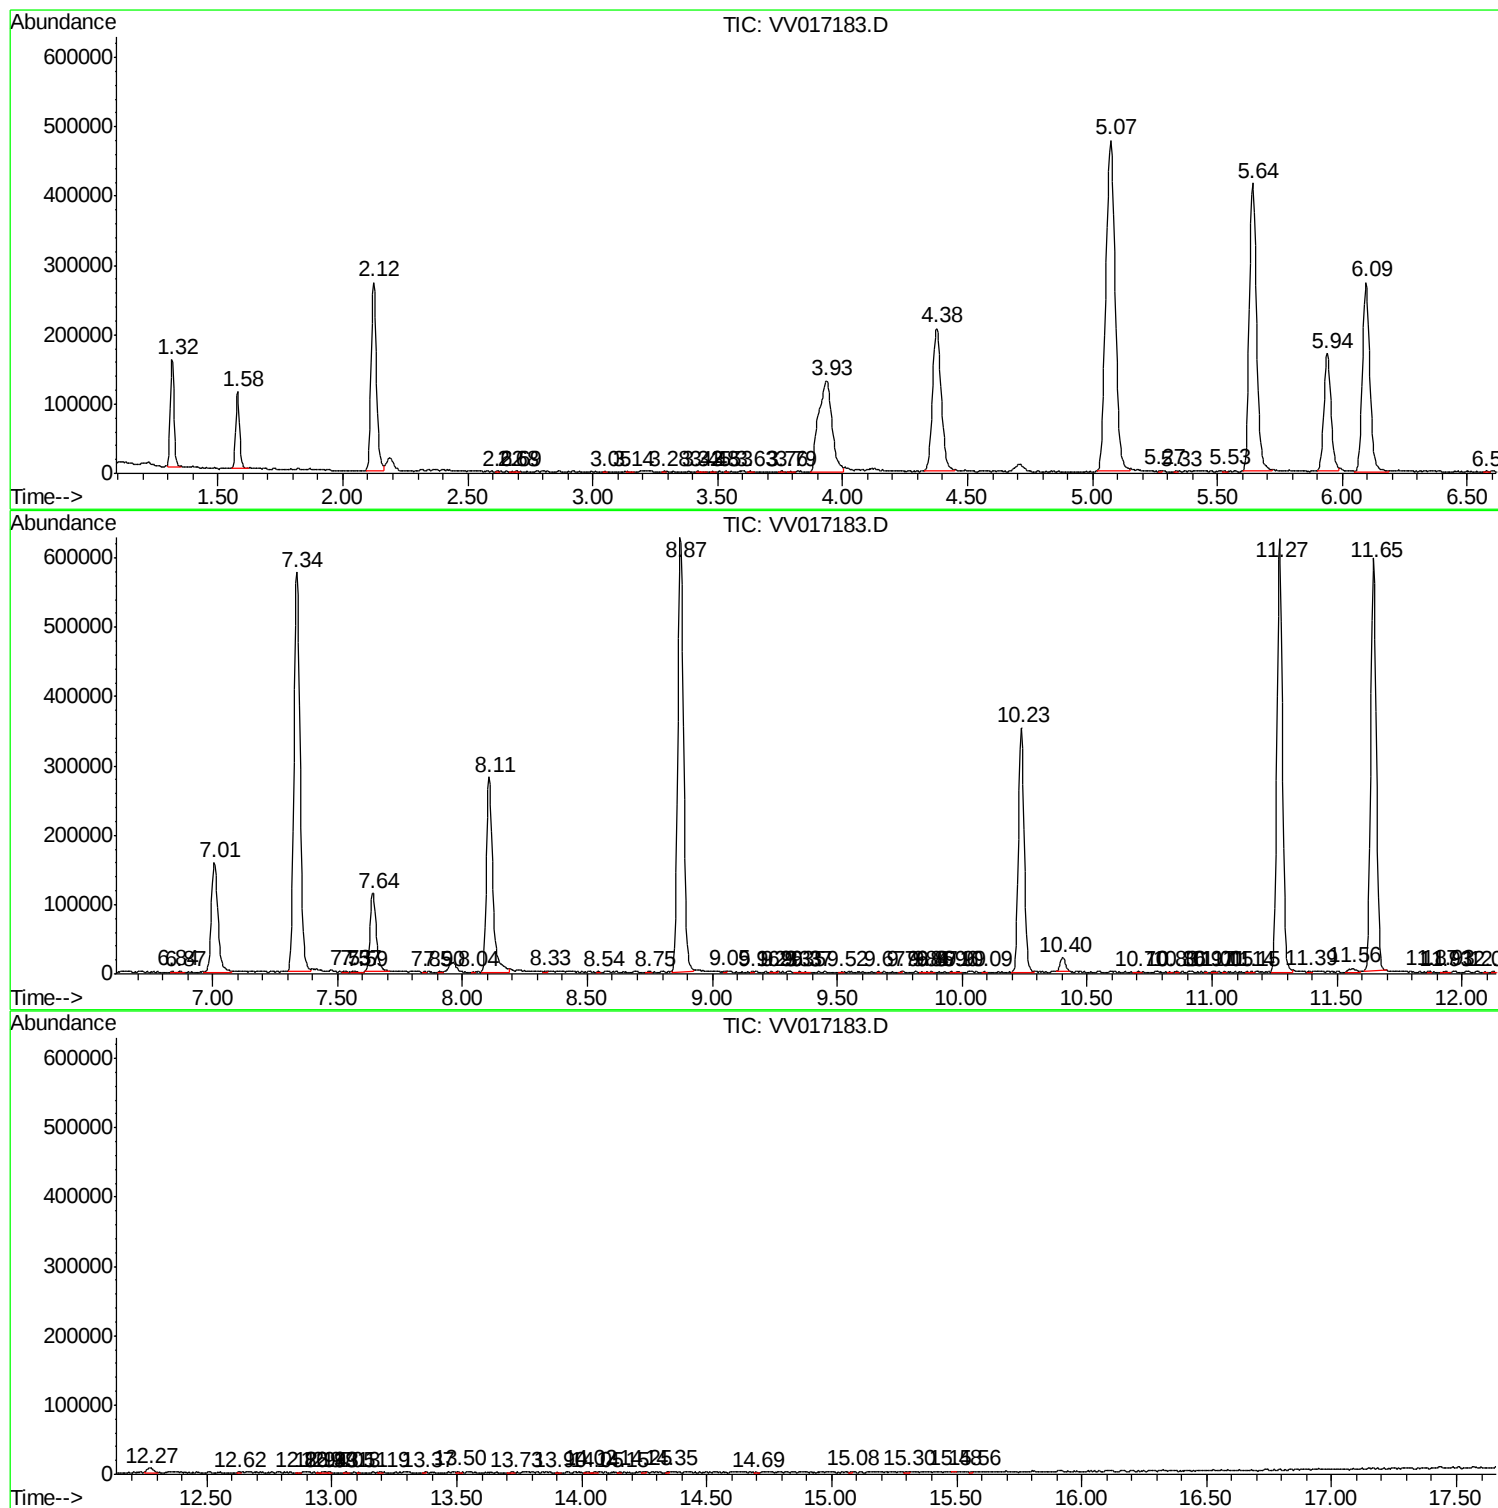

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017183.D
Acq On : 26 Jun 2020 15:54
Operator : SY/MD
Sample : L3103-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017183.D
Acq On : 26 Jun 2020 15:54
Operator : SY/MD
Sample : L3103-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc