

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017184.D
 Acq On : 26 Jun 2020 16:17
 Operator : SY/MD
 Sample : L3103-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	169602	177020	13.09%	1.663%
2	1.579	145	152	163	rVB	108475	123974	9.17%	1.165%
3	2.122	311	321	333	rBV	293784	440920	32.62%	4.143%
4	2.299	373	376	379	rBV5	1766	1191	0.09%	0.011%
5	2.579	460	463	465	rBV4	1415	812	0.06%	0.008%
6	2.666	487	490	493	rBV4	1435	1093	0.08%	0.010%
7	2.717	504	506	508	rBV3	1349	637	0.05%	0.006%
8	2.872	553	554	558	rVB4	1051	609	0.05%	0.006%
9	2.958	578	581	585	rVB3	1929	1466	0.11%	0.014%
10	3.058	606	612	614	rBV5	1092	1129	0.08%	0.011%
11	3.232	664	666	667	rBV	1255	606	0.04%	0.006%
12	3.749	824	827	830	rVB4	1643	989	0.07%	0.009%
13	3.791	837	840	843	rVB3	1043	640	0.05%	0.006%
14	3.814	843	847	848	rBV4	857	603	0.04%	0.006%
15	3.855	857	860	864	rBV5	875	552	0.04%	0.005%
16	3.907	864	876	880	rBV2	96863	189261	14.00%	1.778%
17	4.222	972	974	976	rBV3	1336	600	0.04%	0.006%
18	4.376	1007	1022	1043	rBV2	223117	544823	40.30%	5.119%
19	4.685	1113	1118	1119	rBV4	1737	1401	0.10%	0.013%
20	5.071	1219	1238	1265	rBV2	518153	1351868	100.00%	12.701%
21	5.405	1340	1342	1344	rBV3	1176	597	0.04%	0.006%
22	5.640	1403	1415	1439	rBV	429796	859788	63.60%	8.078%
23	5.830	1471	1474	1477	rBV4	1717	1358	0.10%	0.013%
24	5.939	1495	1508	1524	rBV	227016	441643	32.67%	4.149%
25	6.093	1543	1556	1578	rBV	298827	604923	44.75%	5.683%
26	6.383	1642	1646	1649	rBV5	1205	1372	0.10%	0.013%
27	6.511	1683	1686	1692	rVB5	1383	1268	0.09%	0.012%
28	6.604	1712	1715	1718	rVB3	1263	880	0.07%	0.008%
29	6.624	1718	1721	1722	rBV3	1879	927	0.07%	0.009%
30	6.801	1774	1776	1777	rBV2	1163	575	0.04%	0.005%
31	6.952	1821	1823	1827	rVB4	1337	670	0.05%	0.006%
32	7.006	1827	1840	1857	rBV	169882	307441	22.74%	2.888%
33	7.219	1903	1906	1913	rBV8	1346	1170	0.09%	0.011%
34	7.338	1931	1943	1963	rBV	621261	1063758	78.69%	9.994%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017184.D
 Acq On : 26 Jun 2020 16:17
 Operator : SY/MD
 Sample : L3103-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.582	2017	2019	2022	rBV3	1170	784	0.06%	0.007%
36	7.640	2029	2037	2055	rBV	123695	204368	15.12%	1.920%
37	7.810	2087	2090	2093	rBV5	1982	1106	0.08%	0.010%
38	7.958	2126	2136	2146	rBV4	5721	11701	0.87%	0.110%
39	8.013	2149	2153	2158	rVB7	1409	1468	0.11%	0.014%
40	8.039	2158	2161	2163	rVB4	1191	690	0.05%	0.006%
41	8.106	2173	2182	2199	rBV	313719	536047	39.65%	5.036%
42	8.463	2289	2293	2295	rBV5	1743	1259	0.09%	0.012%
43	8.495	2301	2303	2307	rBV4	1121	775	0.06%	0.007%
44	8.595	2332	2334	2339	rBV5	1156	630	0.05%	0.006%
45	8.756	2382	2384	2387	rVB3	1213	590	0.04%	0.006%
46	8.871	2408	2420	2444	rBV	654392	1049884	77.66%	9.864%
47	9.010	2462	2463	2467	rBV3	1023	627	0.05%	0.006%
48	9.071	2480	2482	2485	rBV3	1367	795	0.06%	0.007%
49	9.122	2497	2498	2502	rBV3	892	665	0.05%	0.006%
50	9.170	2511	2513	2516	rBV4	1454	748	0.06%	0.007%
51	9.231	2530	2532	2535	rBV2	950	603	0.04%	0.006%
52	9.292	2548	2551	2553	rVV4	1357	983	0.07%	0.009%
53	9.344	2565	2567	2572	rVB5	1067	694	0.05%	0.007%
54	9.469	2603	2606	2609	rBV4	1034	795	0.06%	0.007%
55	9.694	2675	2676	2678	rBV2	1049	505	0.04%	0.005%
56	9.900	2735	2740	2742	rBV4	1624	1436	0.11%	0.013%
57	9.984	2763	2766	2768	rBV4	1129	590	0.04%	0.006%
58	10.000	2768	2771	2774	rVB4	1240	792	0.06%	0.007%
59	10.087	2795	2798	2802	rBV4	1172	888	0.07%	0.008%
60	10.122	2806	2809	2811	rBV3	1574	1003	0.07%	0.009%
61	10.238	2830	2845	2864	rBV	391334	619774	45.85%	5.823%
62	10.309	2864	2867	2874	rVV8	2094	2607	0.19%	0.024%
63	10.344	2874	2878	2882	rVB7	1139	1030	0.08%	0.010%
64	10.405	2887	2897	2905	rBV4	7953	14380	1.06%	0.135%
65	10.662	2974	2977	2979	rBV4	1060	758	0.06%	0.007%
66	10.833	3028	3030	3032	rVB3	1156	562	0.04%	0.005%
67	10.849	3032	3035	3036	rBV2	1433	885	0.07%	0.008%
68	10.955	3064	3068	3071	rVB4	1215	822	0.06%	0.008%
69	11.161	3130	3132	3133	rBV2	1148	523	0.04%	0.005%
70	11.270	3155	3166	3182	rBV	655135	986460	72.97%	9.268%
71	11.376	3197	3199	3203	rBV4	1600	1114	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017184.D
 Acq On : 26 Jun 2020 16:17
 Operator : SY/MD
 Sample : L3103-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.556	3244	3255	3264	rBV6	11025	22303	1.65%	0.210%
73	11.646	3271	3283	3302	rBV	646922	1016652	75.20%	9.552%
74	11.797	3324	3330	3333	rBV6	1959	1943	0.14%	0.018%
75	11.948	3373	3377	3379	rBV3	1397	934	0.07%	0.009%
76	11.987	3387	3389	3391	rBV3	1158	511	0.04%	0.005%
77	12.006	3394	3395	3400	rVV5	1069	882	0.07%	0.008%
78	12.077	3415	3417	3419	rBV3	1286	792	0.06%	0.007%
79	12.112	3425	3428	3432	rBV5	1819	1523	0.11%	0.014%
80	12.263	3471	3475	3476	rBV3	2837	1898	0.14%	0.018%
81	12.424	3523	3525	3528	rBV2	1491	1040	0.08%	0.010%
82	12.579	3571	3573	3577	rVB5	1386	853	0.06%	0.008%
83	12.730	3617	3620	3623	rBV4	1428	1001	0.07%	0.009%
84	12.868	3660	3663	3666	rVB5	1233	780	0.06%	0.007%
85	12.942	3682	3686	3689	rBV4	1293	1032	0.08%	0.010%
86	12.980	3692	3698	3701	rBV7	1297	1432	0.11%	0.013%
87	13.058	3718	3722	3723	rBV3	1840	1153	0.09%	0.011%
88	13.115	3737	3740	3741	rBV2	1377	776	0.06%	0.007%
89	13.479	3851	3853	3859	rVB6	1611	1410	0.10%	0.013%
90	13.505	3859	3861	3864	rVB4	1622	688	0.05%	0.006%
91	13.540	3864	3872	3876	rVB8	1720	2831	0.21%	0.027%
92	13.807	3952	3955	3957	rBV4	946	621	0.05%	0.006%
93	13.890	3979	3981	3983	rBV3	1429	760	0.06%	0.007%
94	13.974	4003	4007	4008	rBV4	1368	857	0.06%	0.008%
95	14.414	4142	4144	4147	rBV3	901	624	0.05%	0.006%
96	14.495	4166	4169	4171	rBV5	1083	780	0.06%	0.007%
97	14.668	4219	4223	4224	rBV3	913	626	0.05%	0.006%
98	15.019	4329	4332	4335	rBV3	1576	1231	0.09%	0.012%
99	15.180	4379	4382	4385	rBV5	1360	811	0.06%	0.008%
100	15.517	4484	4487	4490	rBV5	1455	1010	0.07%	0.009%


Sum of corrected areas: 10643659

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017184.D
Acq On : 26 Jun 2020 16:17
Operator : SY/MD
Sample : L3103-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

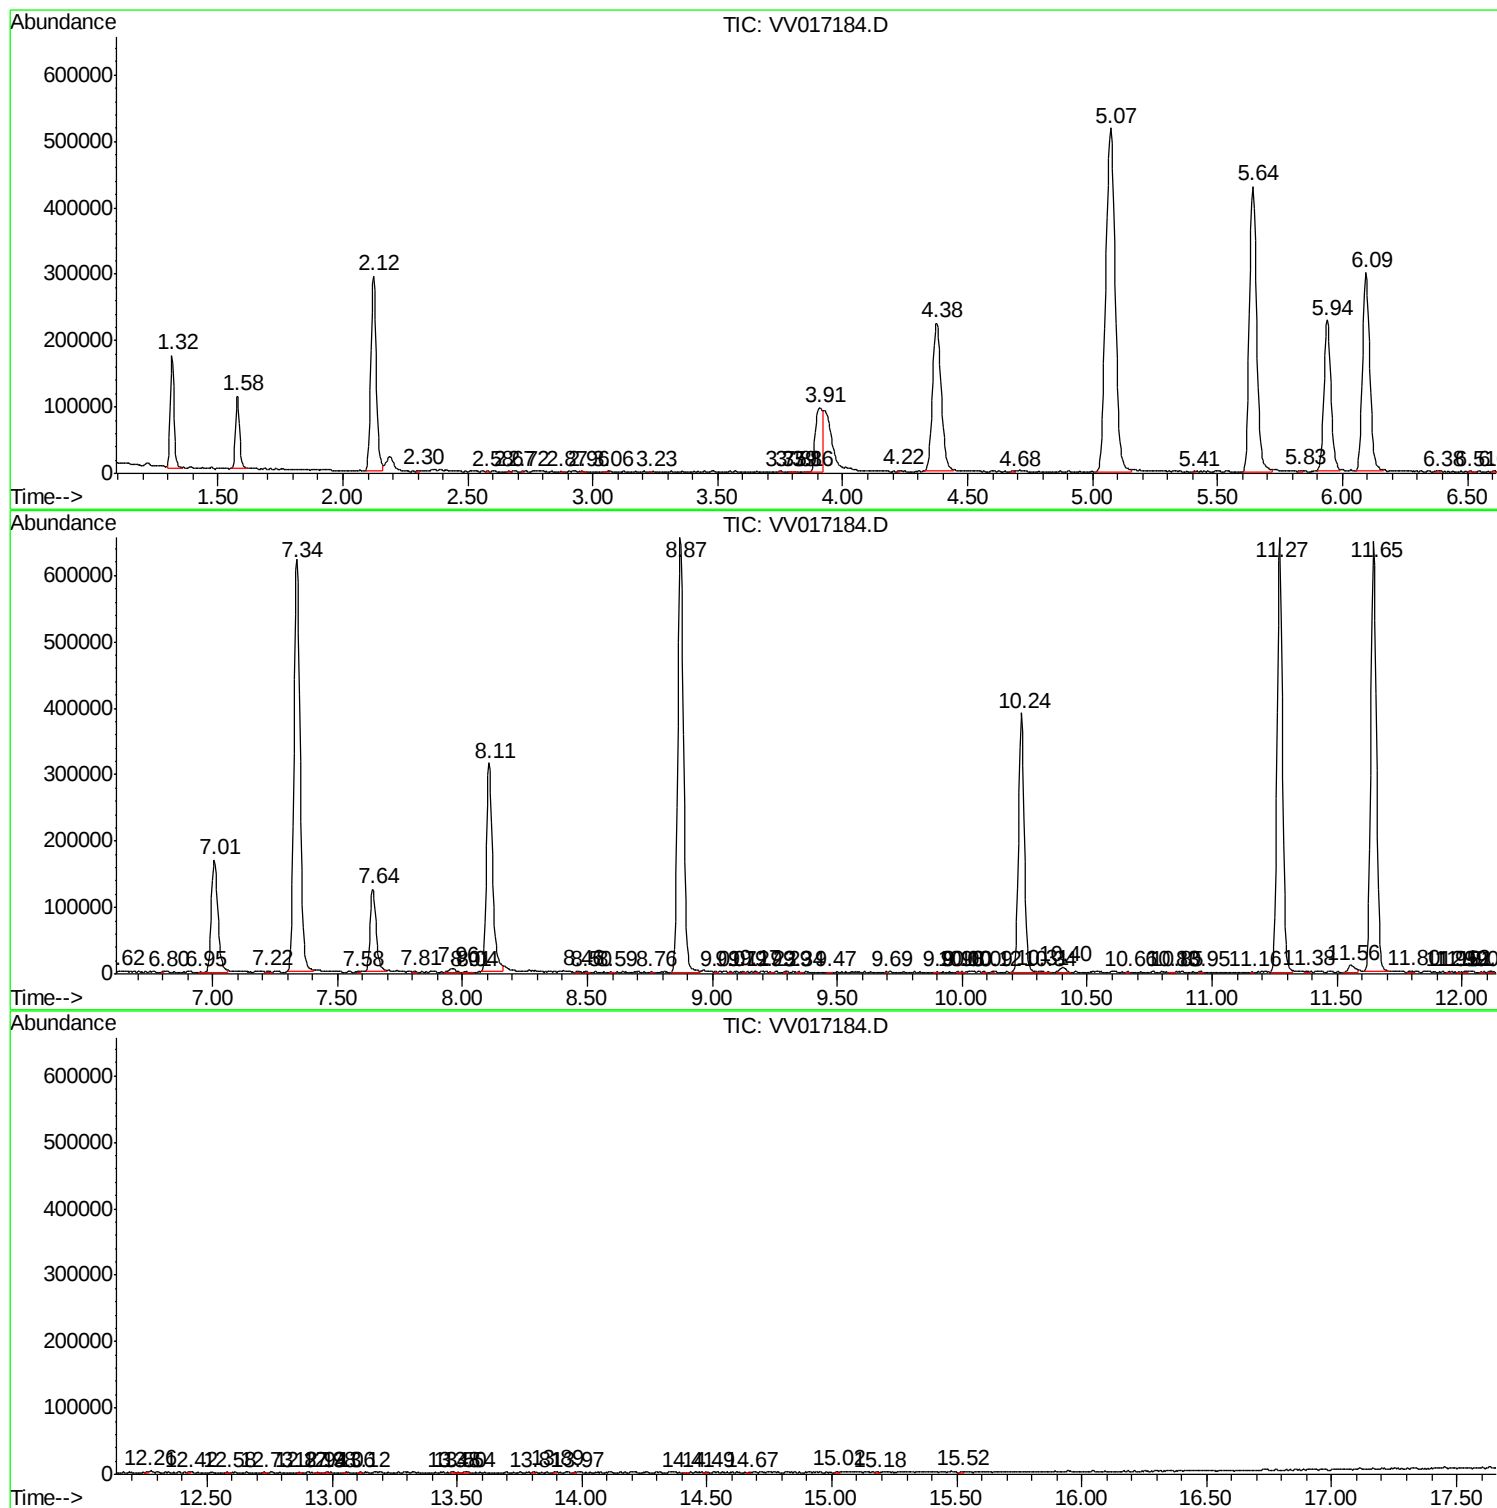

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017184.D
Acq On : 26 Jun 2020 16:17
Operator : SY/MD
Sample : L3103-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q09

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017184.D
Acq On : 26 Jun 2020 16:17
Operator : SY/MD
Sample : L3103-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q09

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
