

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017190.D
 Acq On : 26 Jun 2020 18:36
 Operator : SY/MD
 Sample : L3103-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	163197	170795	13.14%	1.684%
2	1.579	146	152	161	rVB	125874	138179	10.63%	1.363%
3	2.123	311	321	344	rBV	282587	426404	32.82%	4.205%
4	3.036	596	605	609	rBV9	2195	2705	0.21%	0.027%
5	3.071	613	616	617	rBV3	1108	611	0.05%	0.006%
6	3.222	659	663	664	rBV3	1487	955	0.07%	0.009%
7	3.283	677	682	685	rBV6	1434	1350	0.10%	0.013%
8	3.434	723	729	734	rBV8	1213	1546	0.12%	0.015%
9	3.553	761	766	772	rVB9	1321	1383	0.11%	0.014%
10	3.602	779	781	787	rBV5	825	815	0.06%	0.008%
11	3.682	803	806	809	rBV5	990	738	0.06%	0.007%
12	3.727	818	820	824	rVB5	1022	693	0.05%	0.007%
13	3.817	845	848	851	rBV4	1082	659	0.05%	0.006%
14	3.917	866	879	908	rBV	86940	285001	21.93%	2.811%
15	4.203	966	968	970	rBV2	1215	606	0.05%	0.006%
16	4.376	1006	1022	1046	rVV	217391	532767	41.00%	5.254%
17	4.650	1106	1107	1109	rBV2	1235	632	0.05%	0.006%
18	4.756	1139	1140	1145	rVB4	1541	905	0.07%	0.009%
19	4.798	1148	1153	1157	rBV6	1254	1260	0.10%	0.012%
20	4.846	1166	1168	1172	rBV5	888	615	0.05%	0.006%
21	4.897	1181	1184	1187	rBV3	1028	897	0.07%	0.009%
22	4.913	1187	1189	1194	rVB6	1663	1296	0.10%	0.013%
23	4.942	1194	1198	1202	rVB7	1441	1300	0.10%	0.013%
24	4.971	1202	1207	1211	rBV7	1956	1496	0.12%	0.015%
25	5.074	1221	1239	1264	rBV2	506920	1299408	100.00%	12.814%
26	5.322	1314	1316	1317	rBV2	1629	753	0.06%	0.007%
27	5.470	1359	1362	1366	rVB3	1795	1312	0.10%	0.013%
28	5.502	1366	1372	1374	rBV7	1863	2103	0.16%	0.021%
29	5.640	1401	1415	1434	rBV	430553	861169	66.27%	8.493%
30	5.868	1483	1486	1491	rBV7	1641	2038	0.16%	0.020%
31	5.939	1497	1508	1524	rVB6	43869	94074	7.24%	0.928%
32	6.016	1530	1532	1538	rVB6	2217	1575	0.12%	0.016%
33	6.093	1543	1556	1581	rVV	288561	588704	45.31%	5.806%
34	6.354	1633	1637	1639	rBV4	1235	1045	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017190.D
 Acq On : 26 Jun 2020 18:36
 Operator : SY/MD
 Sample : L3103-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.540	1694	1695	1699	rVB3	1202	575	0.04%	0.006%
36	6.589	1708	1710	1712	rBV2	1901	950	0.07%	0.009%
37	6.807	1776	1778	1782	rBV3	1563	1230	0.09%	0.012%
38	7.007	1829	1840	1856	rBV	162305	290155	22.33%	2.861%
39	7.338	1931	1943	1971	rVV	601428	1035757	79.71%	10.214%
40	7.643	2028	2038	2056	rVV	117657	205095	15.78%	2.023%
41	8.010	2149	2152	2153	rBV3	1765	1027	0.08%	0.010%
42	8.109	2171	2183	2203	rBV	303960	542496	41.75%	5.350%
43	8.441	2283	2286	2289	rBV2	1240	911	0.07%	0.009%
44	8.640	2344	2348	2351	rBV4	1769	1397	0.11%	0.014%
45	8.656	2351	2353	2358	rVV5	1338	1078	0.08%	0.011%
46	8.736	2376	2378	2382	rBV2	1353	1014	0.08%	0.010%
47	8.871	2408	2420	2442	rBV	645613	1045857	80.49%	10.314%
48	9.135	2499	2502	2505	rBV4	1355	624	0.05%	0.006%
49	9.154	2505	2508	2509	rBV3	1074	583	0.04%	0.006%
50	9.261	2538	2541	2543	rBV3	907	612	0.05%	0.006%
51	9.733	2686	2688	2692	rVB4	1315	938	0.07%	0.009%
52	9.868	2725	2730	2734	rVB7	1611	1367	0.11%	0.013%
53	9.971	2757	2762	2766	rBV7	1706	1665	0.13%	0.016%
54	10.129	2807	2811	2812	rBV3	1517	1089	0.08%	0.011%
55	10.238	2831	2845	2860	rBV	381815	597751	46.00%	5.895%
56	10.537	2935	2938	2940	rVV3	1931	938	0.07%	0.009%
57	10.553	2940	2943	2946	rBV5	1141	702	0.05%	0.007%
58	10.598	2955	2957	2961	rVB3	1230	605	0.05%	0.006%
59	10.720	2992	2995	2999	rBV6	1185	604	0.05%	0.006%
60	10.740	2999	3001	3005	rBV4	1037	673	0.05%	0.007%
61	10.785	3012	3015	3018	rBV4	780	688	0.05%	0.007%
62	11.170	3134	3135	3137	rBV2	1177	653	0.05%	0.006%
63	11.196	3141	3143	3146	rVB2	1827	779	0.06%	0.008%
64	11.215	3146	3149	3152	rBV4	1246	967	0.07%	0.010%
65	11.270	3155	3166	3186	rBV	629609	965512	74.30%	9.522%
66	11.646	3271	3283	3298	rBV	628635	974397	74.99%	9.609%
67	11.813	3330	3335	3341	rBV6	2134	2469	0.19%	0.024%
68	11.868	3350	3352	3354	rBV3	929	592	0.05%	0.006%
69	11.913	3363	3366	3369	rVB4	1228	754	0.06%	0.007%
70	11.974	3384	3385	3388	rBV3	949	578	0.04%	0.006%
71	12.170	3443	3446	3448	rBV4	1310	881	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017190.D
 Acq On : 26 Jun 2020 18:36
 Operator : SY/MD
 Sample : L3103-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.196	3451	3454	3457	rBV4	1387	1143	0.09%	0.011%
73	12.257	3470	3473	3475	rBV4	1178	905	0.07%	0.009%
74	12.318	3488	3492	3494	rBV4	1062	692	0.05%	0.007%
75	12.331	3494	3496	3499	rVB2	1059	677	0.05%	0.007%
76	12.386	3511	3513	3516	rBV4	1303	846	0.07%	0.008%
77	12.498	3545	3548	3551	rBV5	1160	769	0.06%	0.008%
78	12.598	3576	3579	3583	rBV4	1263	943	0.07%	0.009%
79	12.675	3595	3603	3608	rBV8	1551	1958	0.15%	0.019%
80	12.733	3619	3621	3624	rBV4	1169	775	0.06%	0.008%
81	12.865	3659	3662	3664	rBV3	1009	683	0.05%	0.007%
82	12.897	3669	3672	3677	rBV6	1450	1465	0.11%	0.014%
83	12.984	3696	3699	3702	rVV4	1535	1009	0.08%	0.010%
84	13.006	3703	3706	3709	rVB5	1597	1000	0.08%	0.010%
85	13.154	3748	3752	3754	rBV3	1001	852	0.07%	0.008%
86	13.286	3790	3793	3797	rBV4	1669	1326	0.10%	0.013%
87	13.395	3823	3827	3828	rBV4	982	622	0.05%	0.006%
88	13.550	3871	3875	3876	rBV2	1264	608	0.05%	0.006%
89	13.749	3932	3937	3938	rBV3	1533	1091	0.08%	0.011%
90	14.096	4041	4045	4047	rBV3	1725	1099	0.08%	0.011%
91	14.727	4237	4241	4243	rBV5	1567	929	0.07%	0.009%
92	14.743	4243	4246	4248	rBV2	1728	1023	0.08%	0.010%
93	14.842	4273	4277	4283	rBV7	2010	3060	0.24%	0.030%
94	14.900	4292	4295	4298	rBV5	1563	1130	0.09%	0.011%
95	15.054	4340	4343	4345	rBV3	1321	794	0.06%	0.008%
96	15.116	4359	4362	4365	rBV4	1338	902	0.07%	0.009%
97	15.260	4401	4407	4409	rBV7	1376	1677	0.13%	0.017%
98	15.318	4423	4425	4427	rBV3	1806	635	0.05%	0.006%
99	15.675	4534	4536	4538	rBV3	1296	590	0.05%	0.006%
100	15.739	4553	4556	4557	rBV2	2338	1309	0.10%	0.013%


Sum of corrected areas: 10140264

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017190.D
Acq On : 26 Jun 2020 18:36
Operator : SY/MD
Sample : L3103-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q19

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

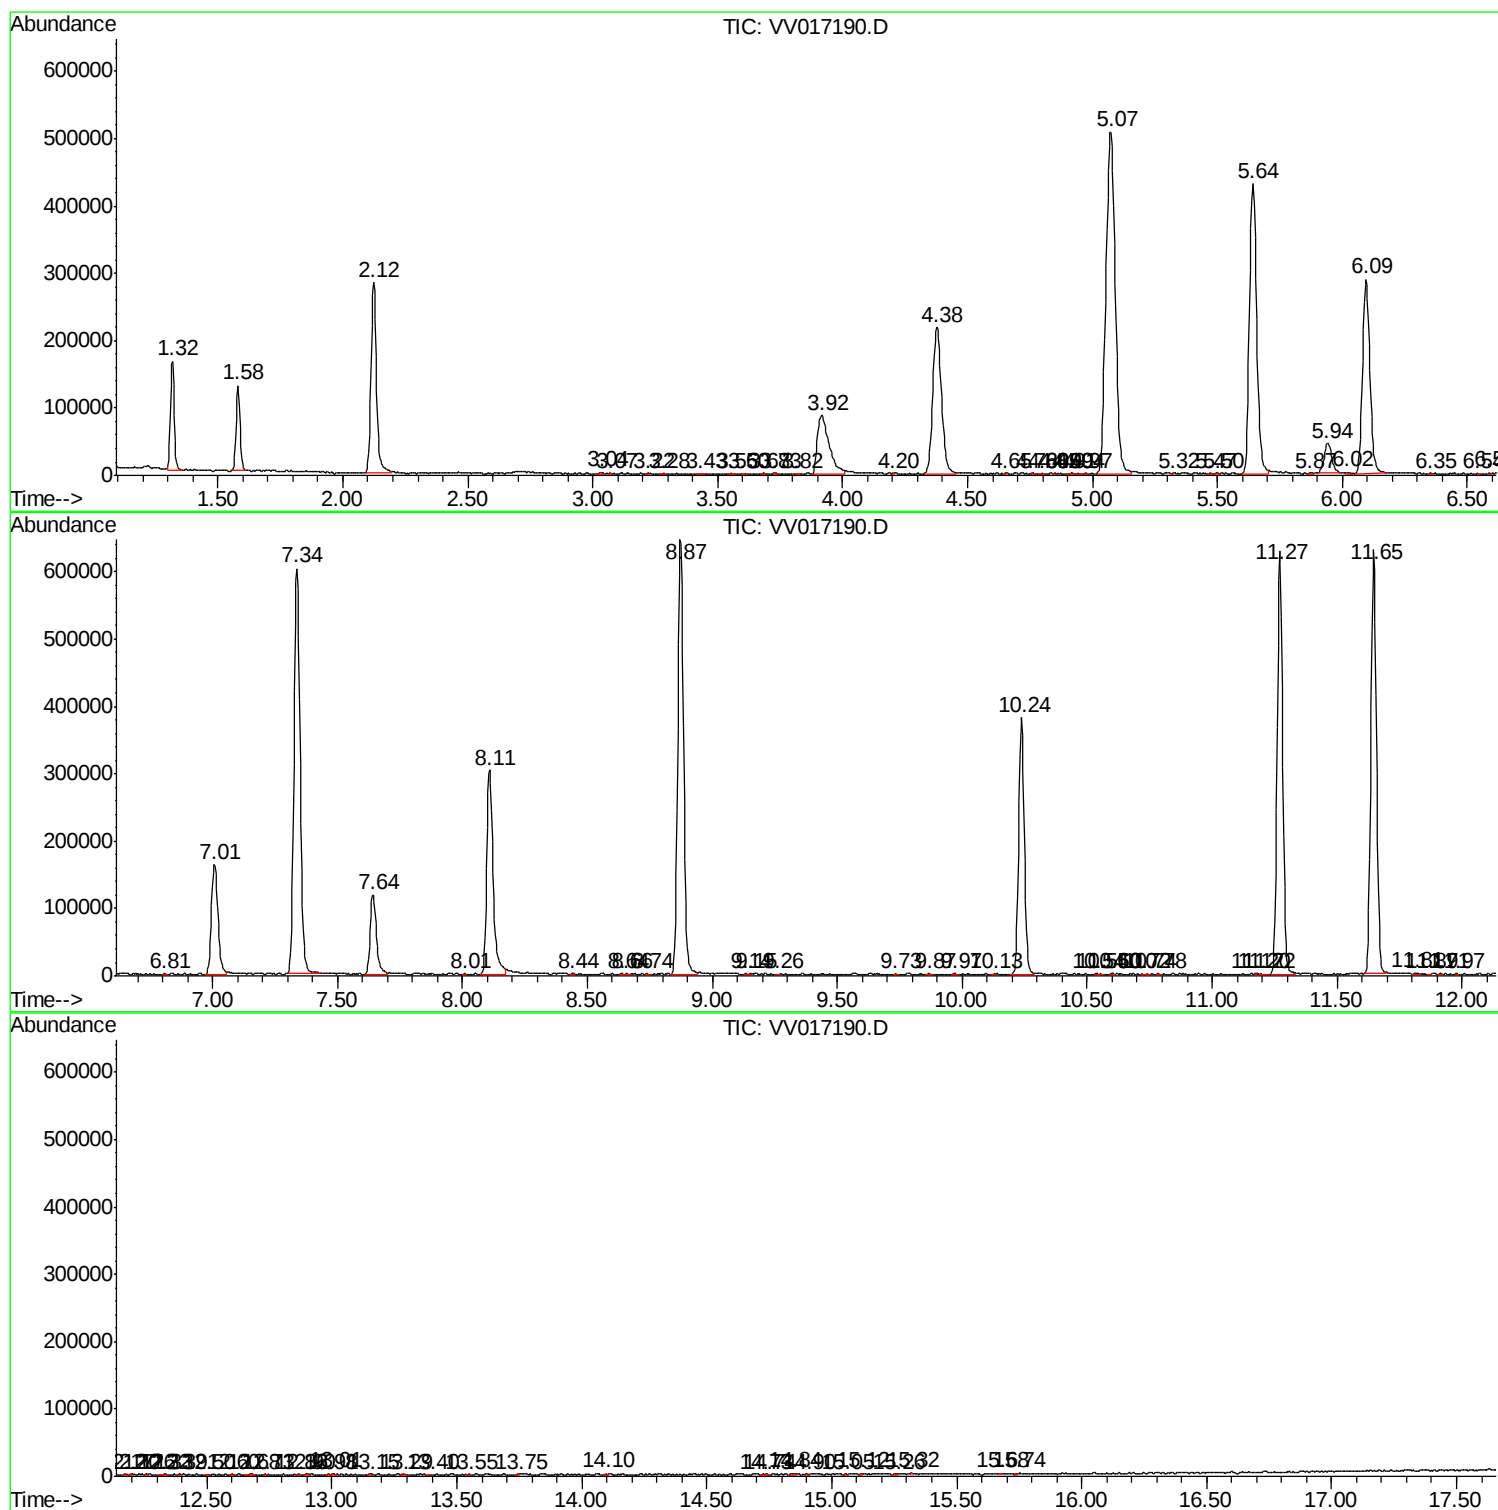

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017190.D
Acq On : 26 Jun 2020 18:36
Operator : SY/MD
Sample : L3103-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q19

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017190.D
Acq On : 26 Jun 2020 18:36
Operator : SY/MD
Sample : L3103-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q19

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc